


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120518\
 Data File : BF111104.D
 Acq On : 5 Dec 2018 13:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 05 17:30:55 2018

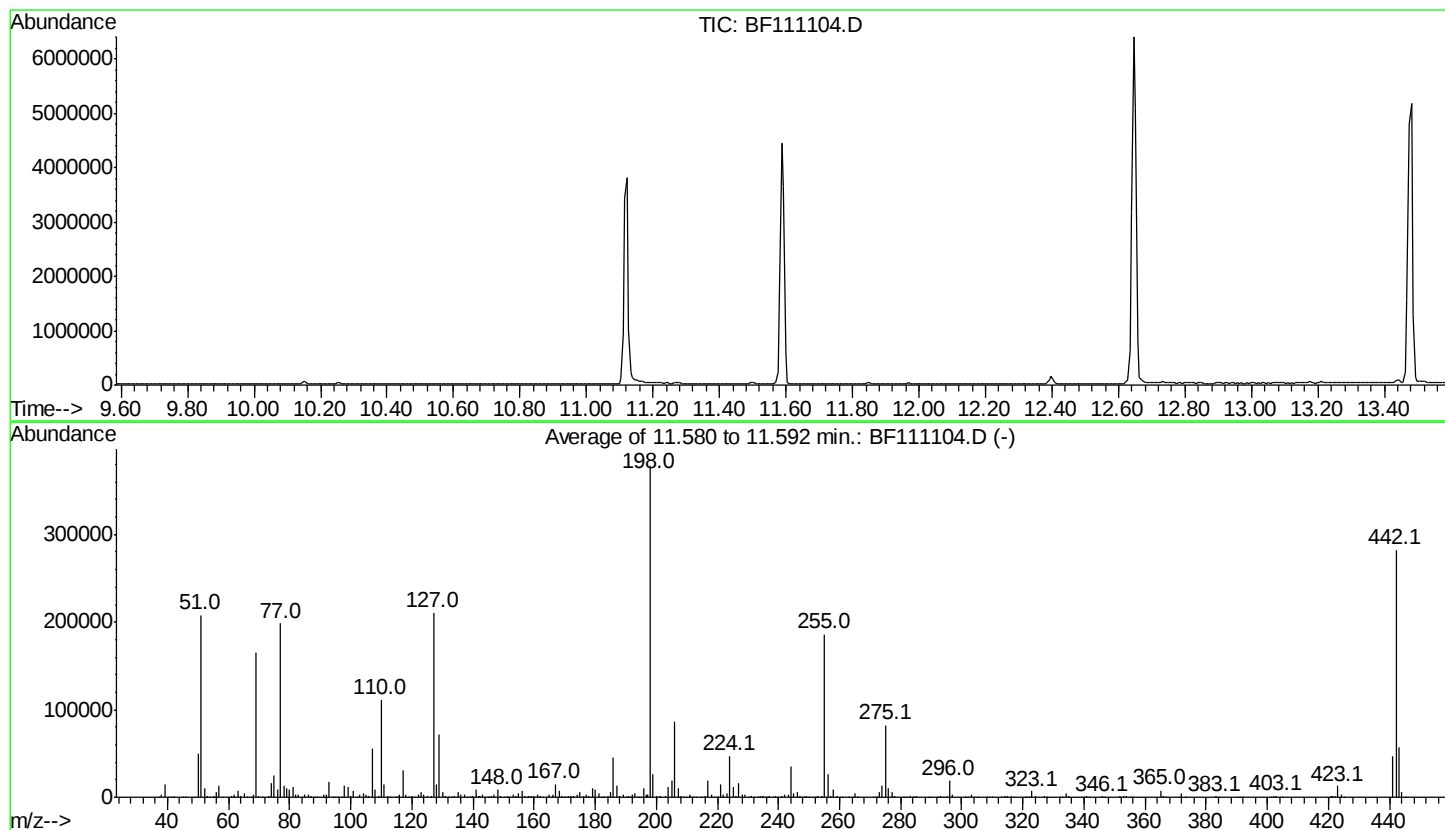

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	208294	PASS
68	69	0.00	2	1.6	2597	PASS
69	198	0.00	100	43.6	165269	PASS
70	69	0.00	2	0.5	868	PASS
127	198	10	80	55.8	211250	PASS
197	198	0.00	2	0.7	2602	PASS
198	198	100	100	100.0	378645	PASS
199	198	5	9	7.0	26504	PASS
275	198	10	60	21.6	81896	PASS
365	198	1	100	2.1	8019	PASS
441	198	0.01	100	12.4	47087	PASS
442	198	50	100	74.5	282168	PASS
443	442	15	24	20.3	57415	PASS