
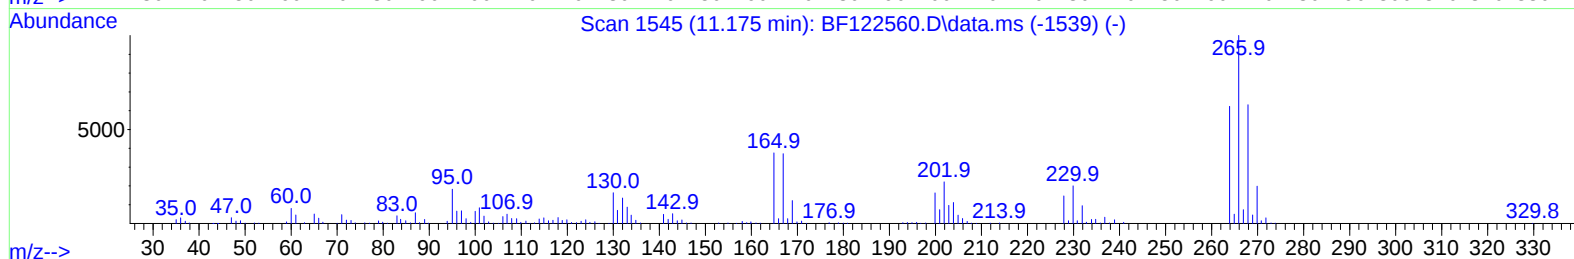
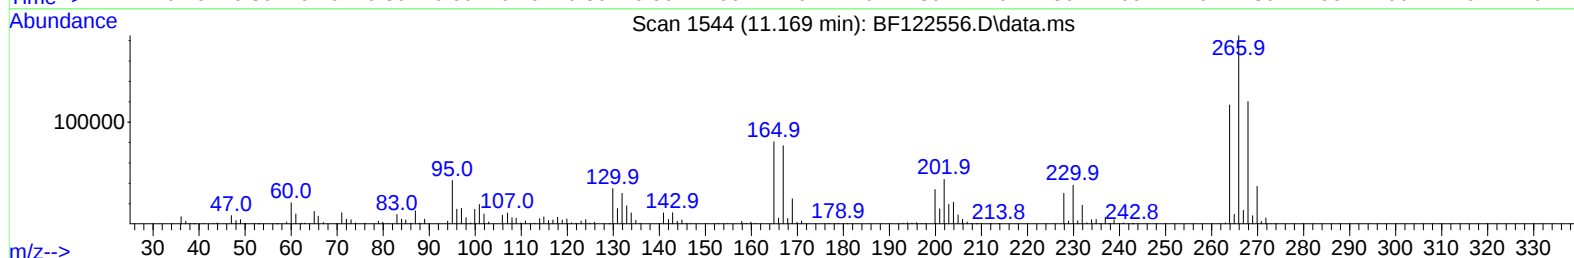


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120520\
Data File : BF122556.D
Acq On : 5 Dec 2020 13:35
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 04:58:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

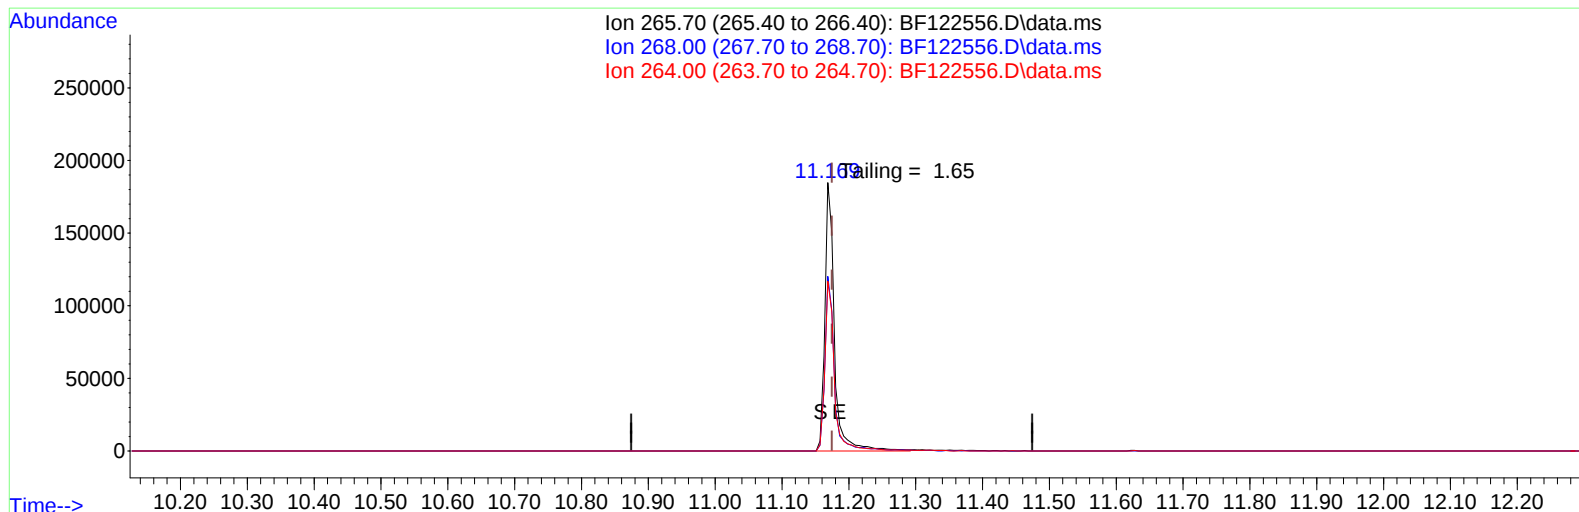

TIC: BF122556.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 33611.90 ng

response 184070

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.08
264.00	62.30	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120520\
Data File : BF122556.D
Acq On : 5 Dec 2020 13:35
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 04:58:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

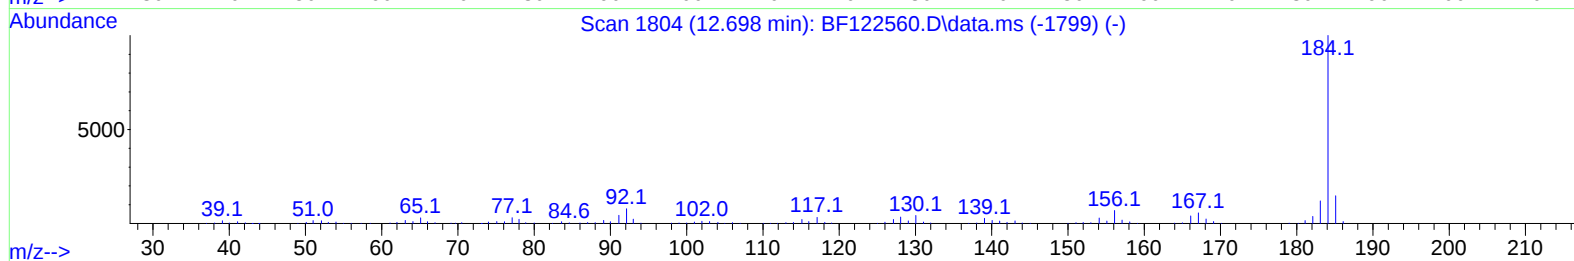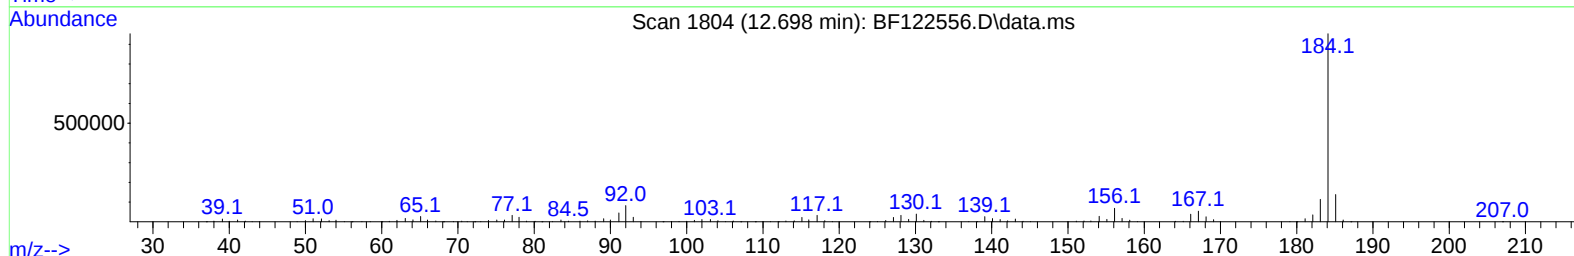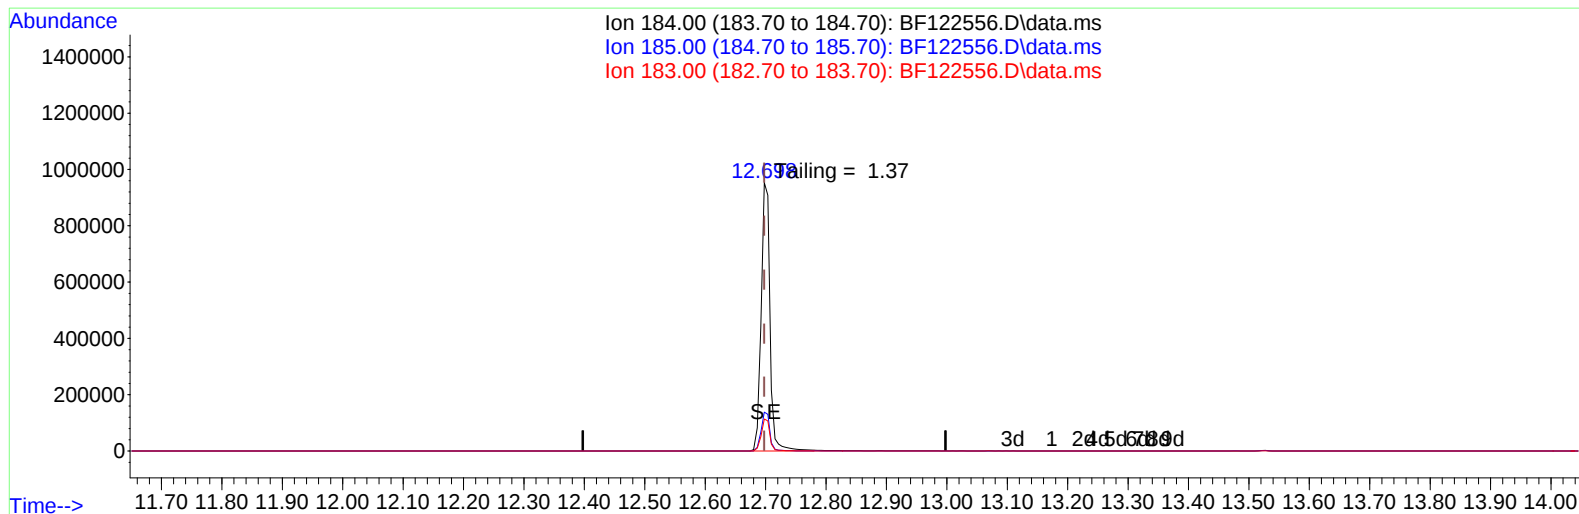

TIC: BF122556.D\data.ms

(77) Benzidine

12.698min (-0.000) 395832.11 ng m

response 984617

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.51
183.00	12.10	11.96
0.00	0.00	0.00