


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120520\
Data File : BF122556.D
Acq On : 5 Dec 2020 13:35
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 07 12:08:49 2020

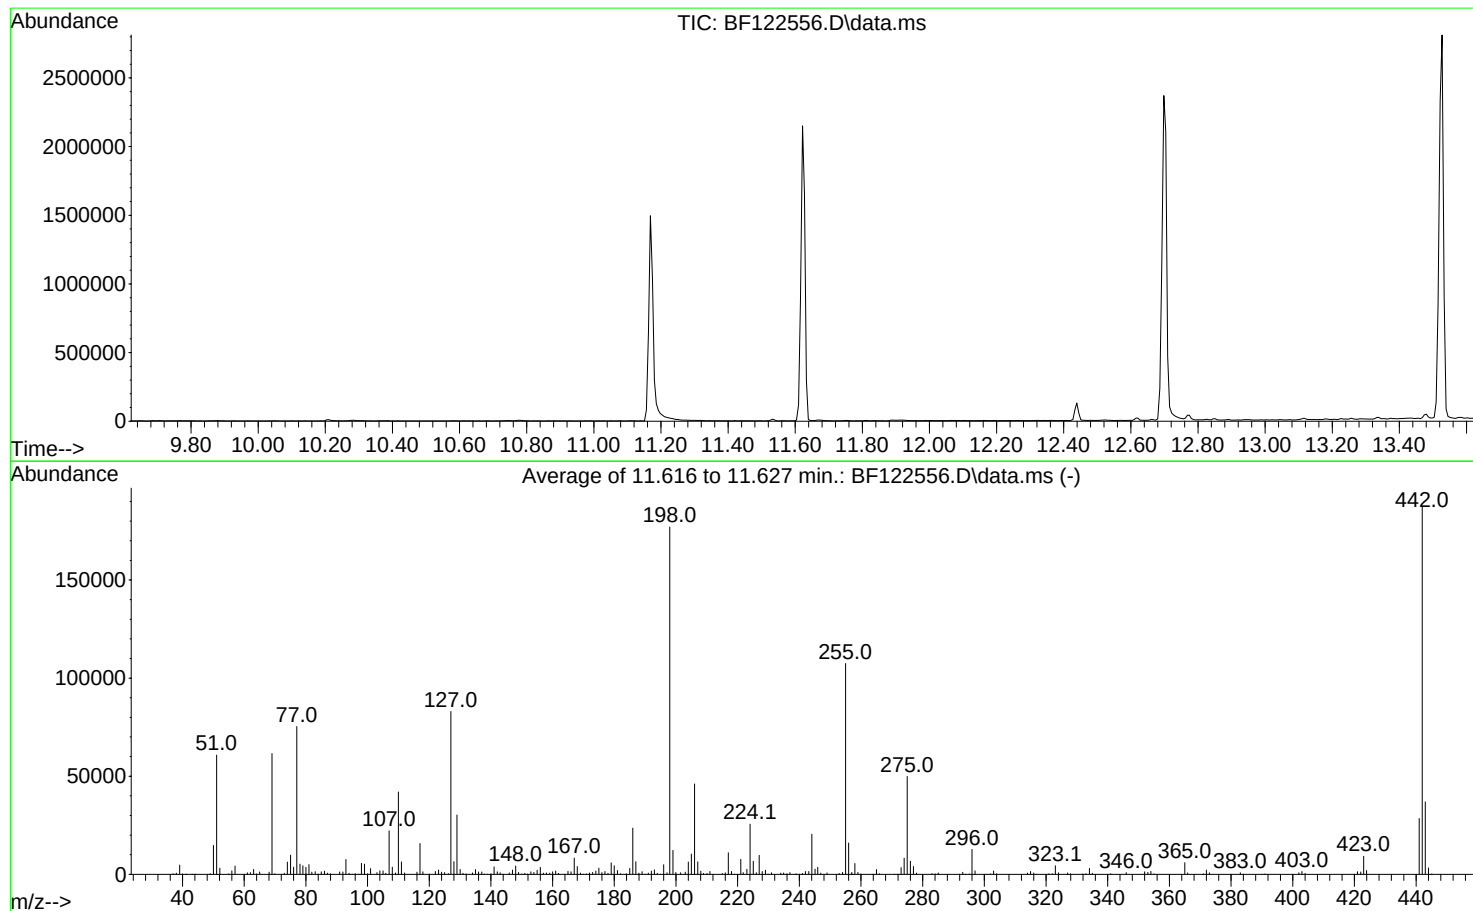

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	60717	PASS
68	69	0.00	2	1.9	1157	PASS
69	198	0.00	100	34.8	61552	PASS
70	69	0.00	2	0.5	293	PASS
127	198	10	80	46.9	83019	PASS
197	198	0.00	2	0.5	798	PASS
198	198	100	100	100.0	176984	PASS
199	198	5	9	6.9	12274	PASS
275	198	10	60	28.2	49885	PASS
365	198	1	100	3.4	5958	PASS
441	198	0.01	100	16.1	28495	PASS
442	442	100	100	100.0	187453	PASS
443	442	15	24	19.7	36921	PASS