
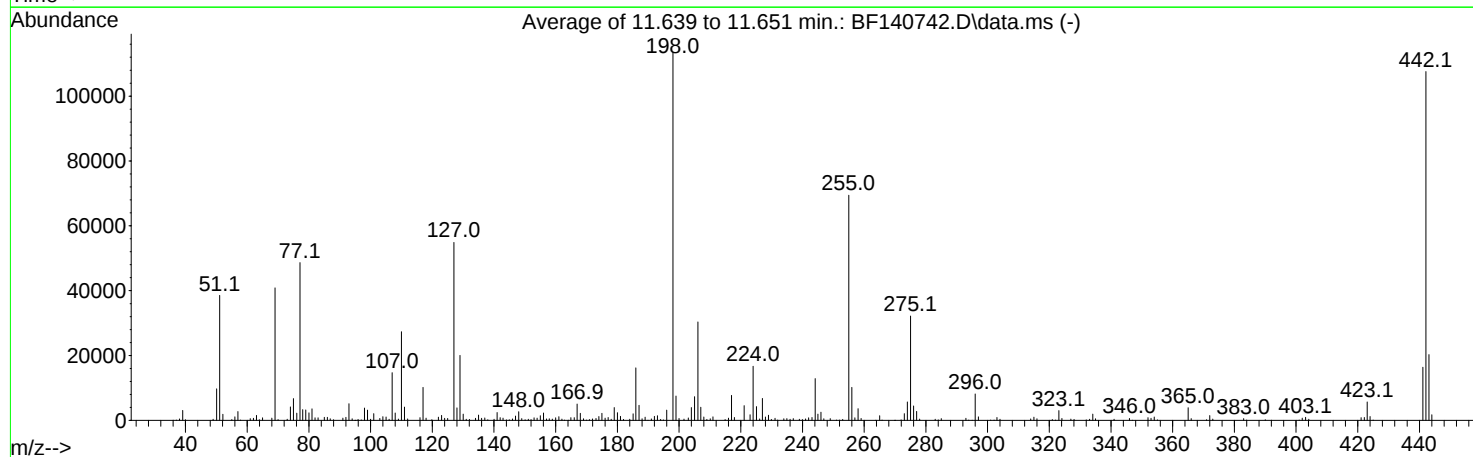


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120524\
Data File : BF140742.D
Acq On : 05 Dec 2024 11:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

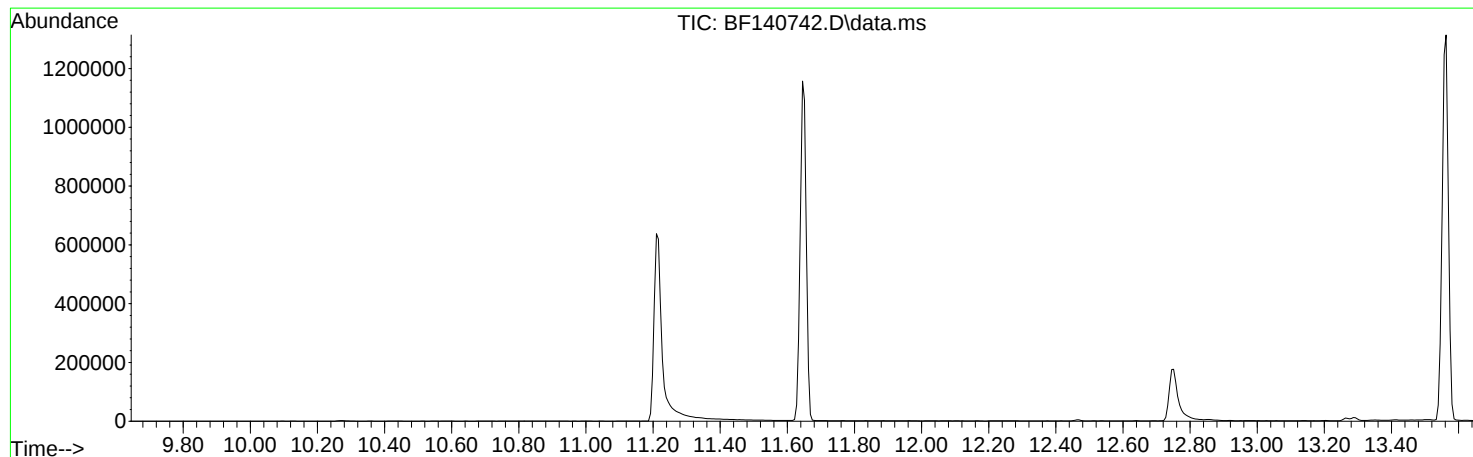

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	38539	PASS
68	69	0.00	2	1.7	682	PASS
69	198	0.00	100	36.0	40883	PASS
70	69	0.00	2	0.7	270	PASS
127	198	10	80	48.4	54901	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	113456	PASS
199	198	5	9	6.6	7520	PASS
275	198	10	60	28.4	32187	PASS
365	198	1	100	3.4	3911	PASS
441	198	0.01	100	14.4	16380	PASS
442	442	50	100	100.0	107592	PASS
443	442	15	24	18.9	20307	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/5/2024	BNA_F	<u>BF140742.D</u>
Compound Name	Response	Retention Time
DDT	343493	13.563
DDD	7766	13.292
DDE	431	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8197	351690	2.33

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120524\
Data File : BF140742.D
Acq On : 05 Dec 2024 11:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 05 12:28:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

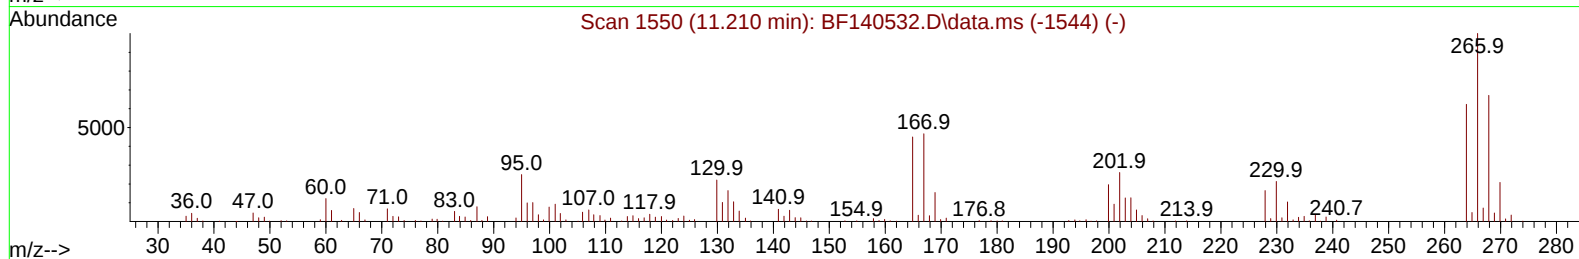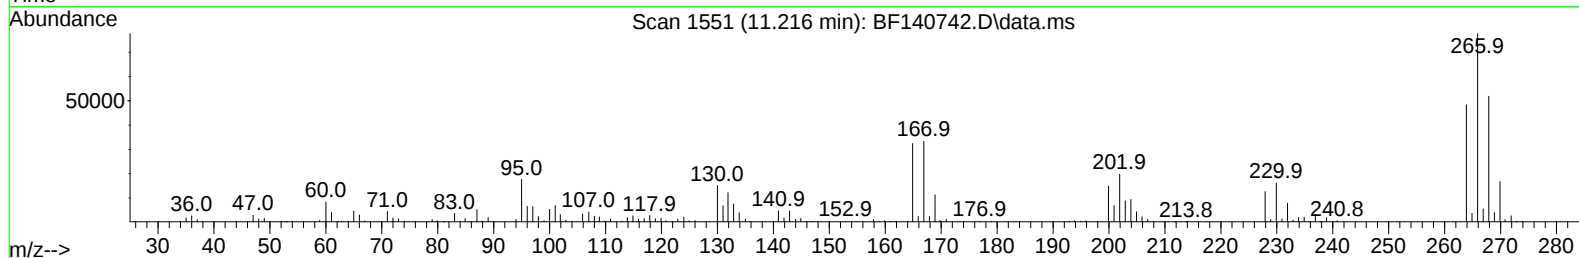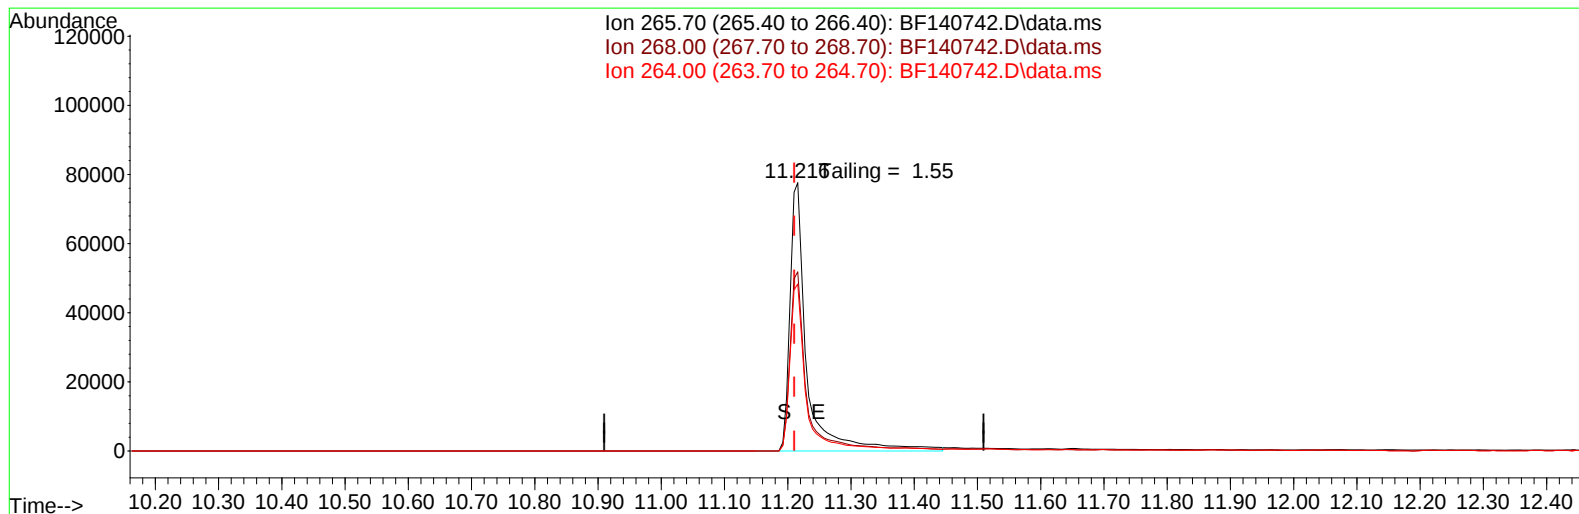

TIC: BF140742.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 504255.93 ng




response 145557

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	66.80
264.00	62.30	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120524\
Data File : BF140742.D
Acq On : 05 Dec 2024 11:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 05 12:28:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

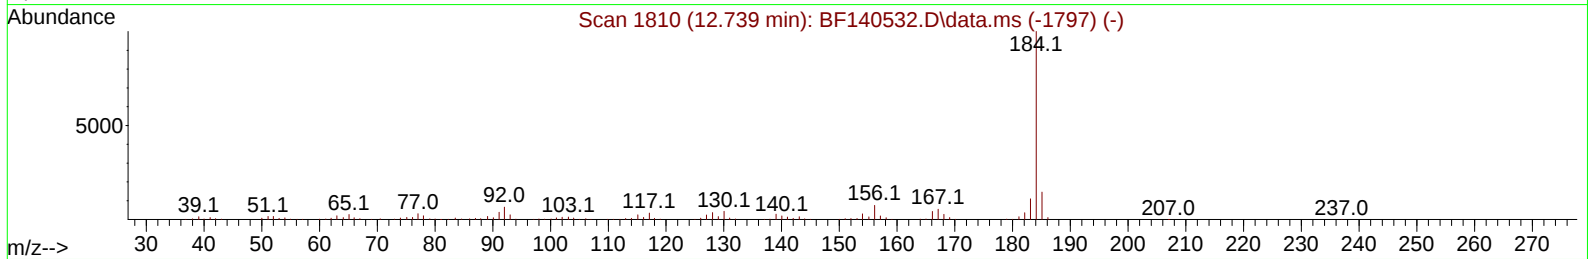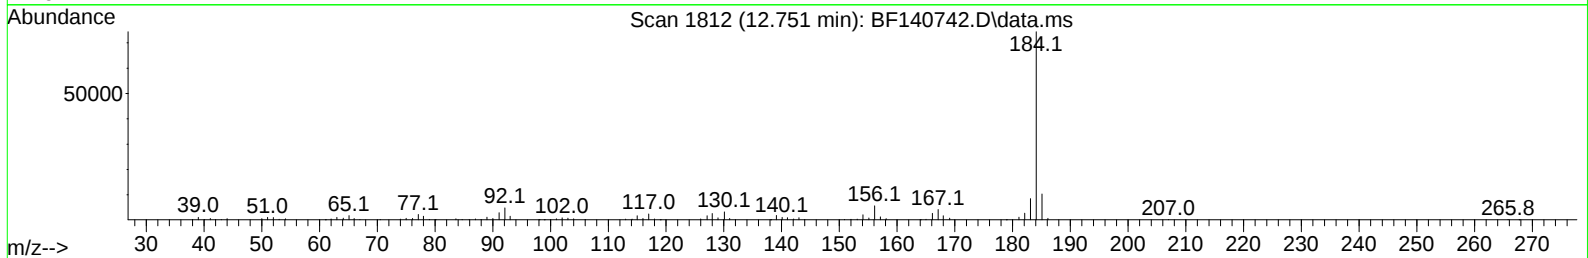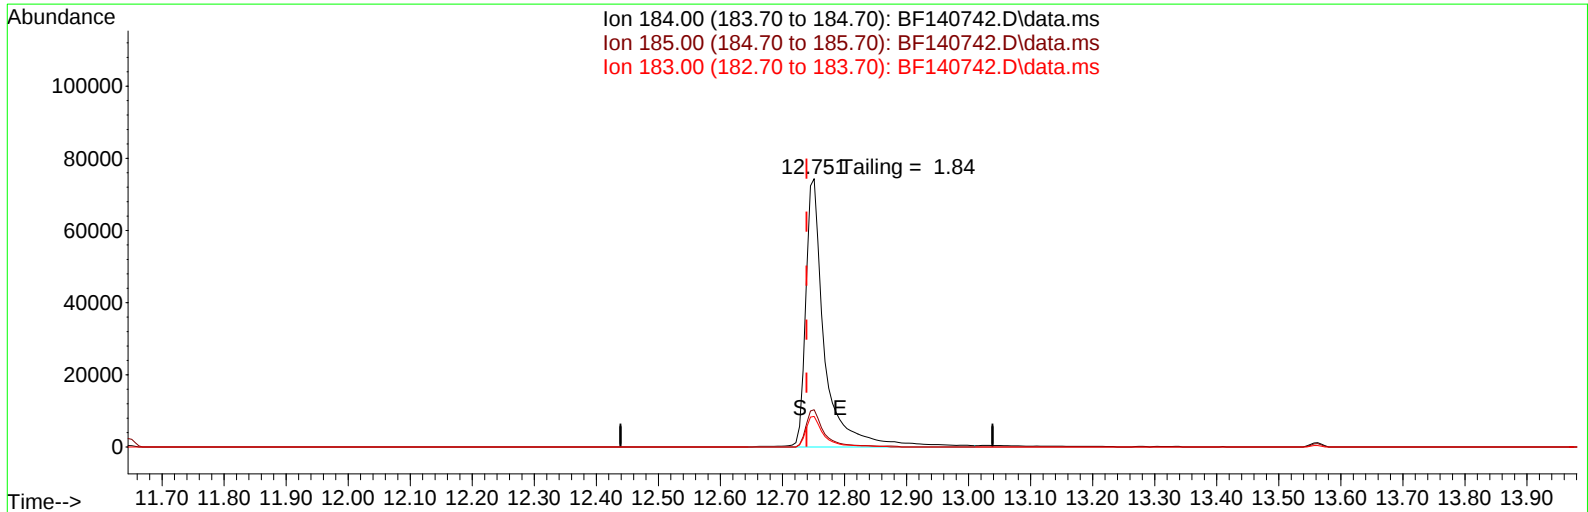

TIC: BF140742.D\data.ms

(77) Benzidine

12.751min (+ 0.012) 0.00 ng

response 158118

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.91
183.00	11.00	11.40
0.00	0.00	0.00