

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120615\
 Data File : BF083556.D
 Acq On : 7 Dec 2015 11:48
 Operator : UM/IZ
 Sample : G4614-01DL 5X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Dec 07 12:47:08 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 05 04:12:46 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.73	152	154448	20.00	ng	-0.03
21) Naphthalene-d8	7.63	136	568449	20.00	ng	-0.05
38) Acenaphthene-d10	10.42	164	262026	20.00	ng	-0.05
63) Phenanthrene-d10	12.82	188	403025	20.00	ng	-0.03
75) Chrysene-d12	17.01	240	340409	20.00	ng	-0.03
86) Perylene-d12	18.65	264	268777	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	4.01	112	298860	29.36	ng	-0.02
7) Phenol-d6	5.30	99	410188	29.24	ng	-0.02
23) Nitrobenzene-d5	6.56	82	254696	20.94	ng	-0.05
41) 2,4,6-Tribromophenol	11.71	330	57026	23.59	ng	-0.05
44) 2-Fluorobiphenyl	9.38	172	374184	19.37	ng	-0.05
78) Terphenyl-d14	15.45	244	245132	16.02	ng	-0.03
Target Compounds						Qvalue
19) n-Nitroso-di-n-propylamine	6.56	70	31634	3.38	ng	# 81
20) 3+4-Methylphenols	6.43	107	40597	3.34	ng	96
31) Naphthalene	7.66	128	61385	2.03	ng	100
32) Benzoic acid	7.46	122	1740	2.97	ng	# 28
49) Dimethylphthalate	10.06	163	81208	3.94	ng	# 98
51) Acenaphthene	10.48	154	61549	3.72	ng	97
54) Dibenzofuran	10.76	168	48733	2.13	ng	95
55) 4-Nitrophenol	10.76	139	18574	7.04	ng	# 9
57) Fluorene	11.31	166	67561	3.39	ng	97
70) Phenanthrene	12.85	178	657099	28.01	ng	99
71) Anthracene	12.95	178	159061	6.65	ng	97
72) Carbazole	13.24	167	58674	2.86	ng	98
74) Fluoranthene	14.79	202	717946	30.88	ng	98
77) Pyrene	15.14	202	617385	24.24	ng	# 95
80) Benzo(a)anthracene	17.00	228	290042	14.56	ng	97
82) Chrysene	17.05	228	274622	13.84	ng	99
85) Indeno(1,2,3-cd)pyrene	19.89	276	84284	4.96	ng	# 100
87) Benzo(b)fluoranthene	18.27	252	339199	22.47	ng	# 96
88) Benzo(k)fluoranthene	18.27	252	339199	21.94	ng	97
89) Benzo(a)pyrene	18.55	252	118752	8.09	ng	97
91) Benzo(g,h,i)perylene	20.26	276	81017	5.69	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120615\
Data File : BF083556.D
Acq On : 7 Dec 2015 11:48
Operator : UM/IZ
Sample : G4614-01DL 5X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :

Quant Time: Dec 07 12:47:08 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 05 04:12:46 2015
Response via : Initial Calibration

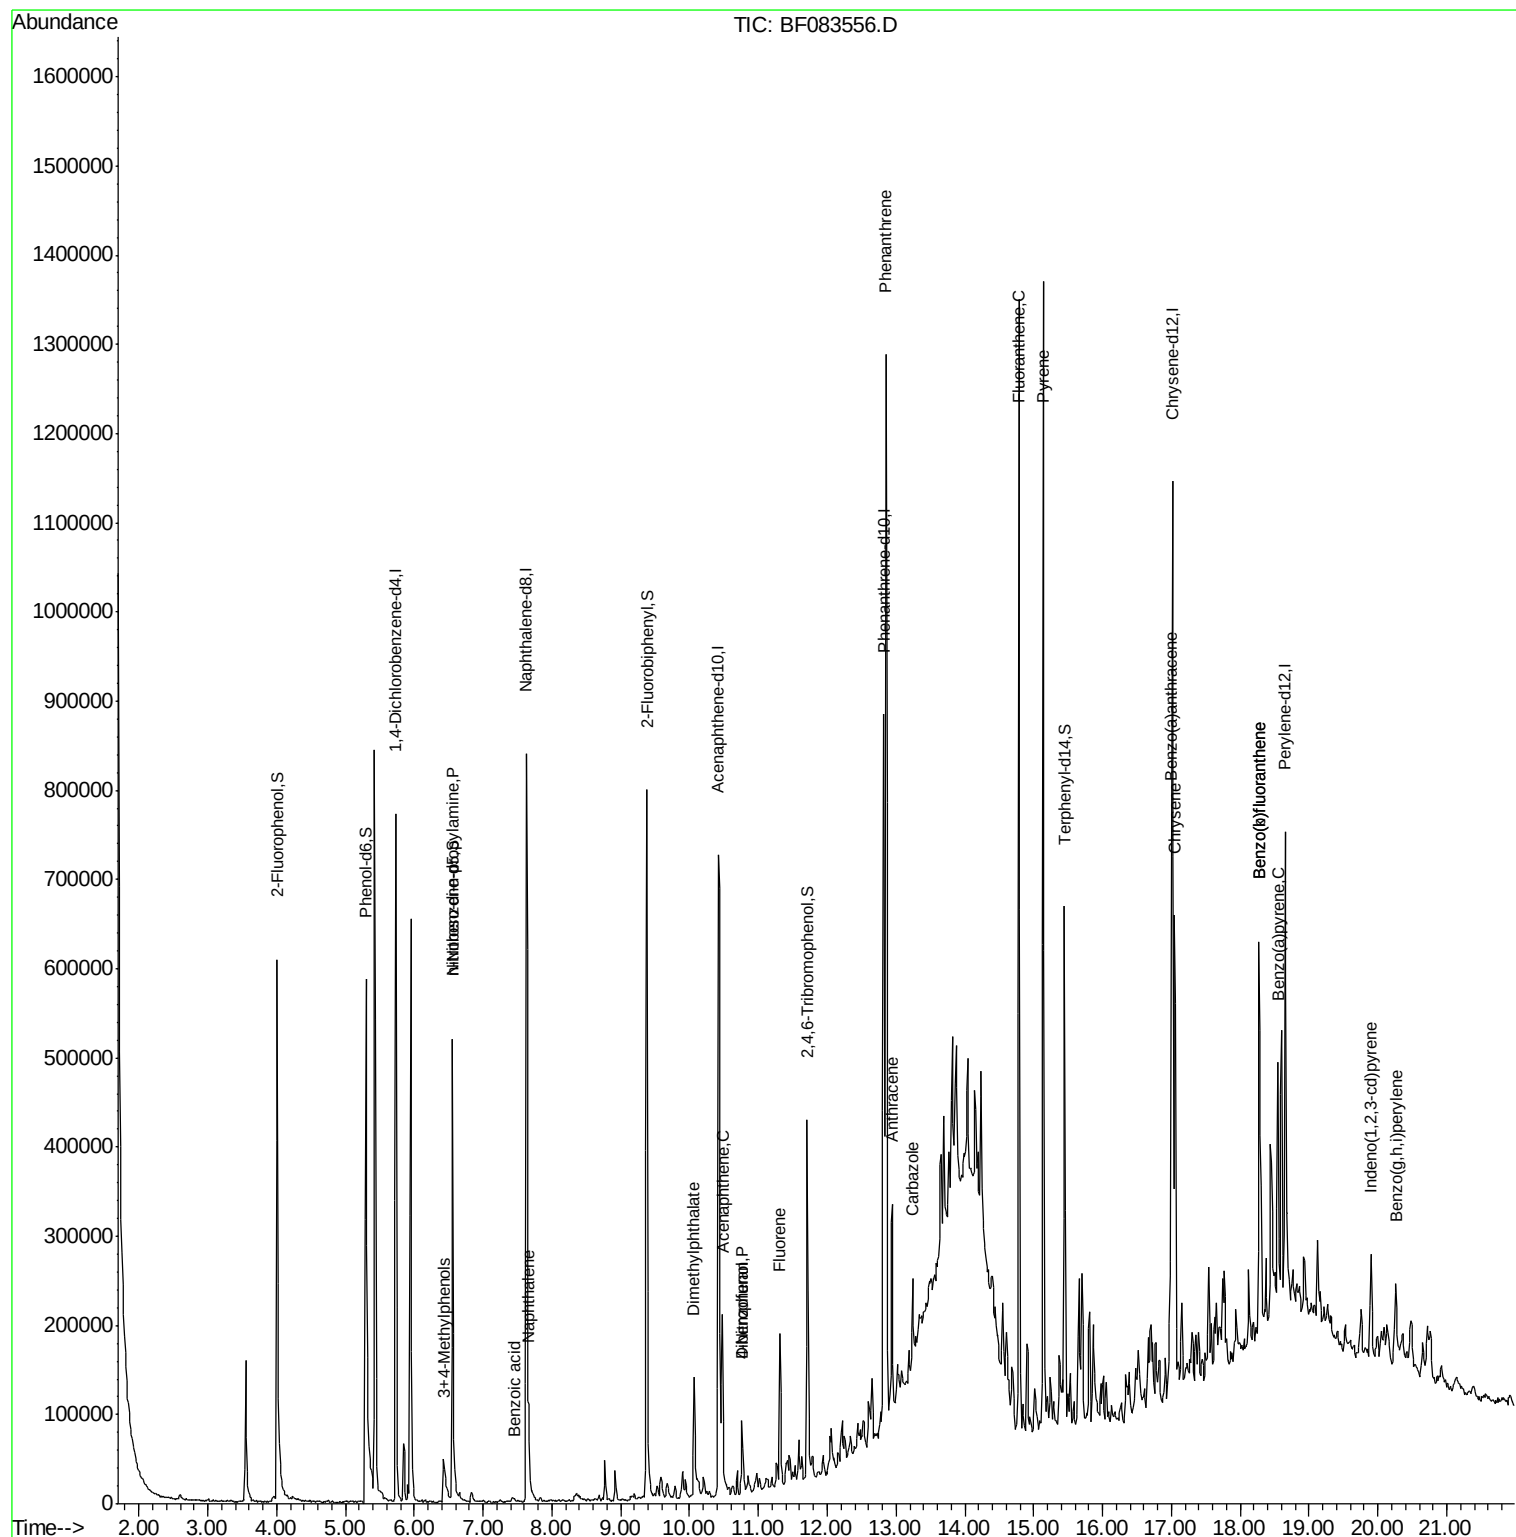




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 5.73 min Scan# 354
Delta R.T. -0.03 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 154448
Ion Ratio Lower Upper
152 100
150 153.8 126.5 189.7
115 60.3 52.3 78.5

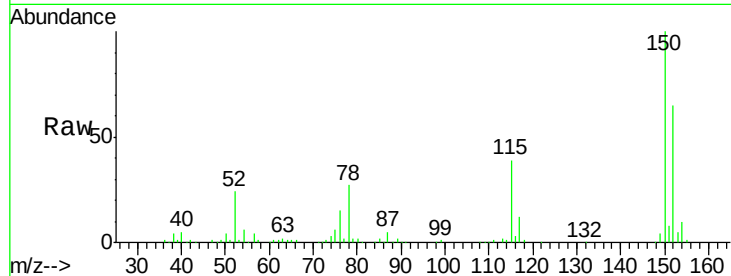


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

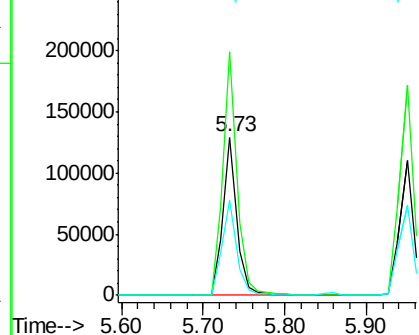



#5


2-Fluorophenol
Concen: 29.36 ng
RT: 4.01 min Scan# 203
Delta R.T. -0.02 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48

Tgt Ion:112 Resp: 298860
Ion Ratio Lower Upper
112 100
64 64.0 50.5 75.7
63 31.7 25.8 38.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

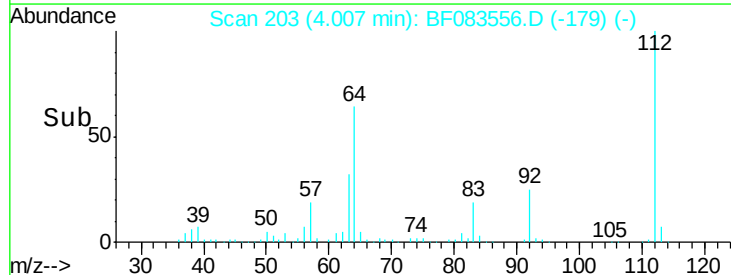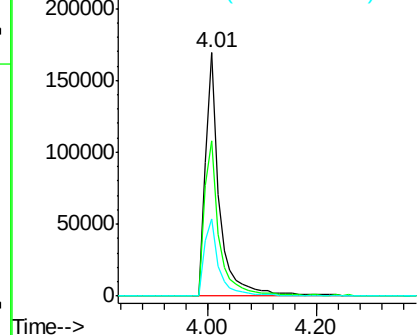



#7

Phenol-d6

Concen: 29.24 ng

RT: 5.30 min Scan# 316

Delta R.T. -0.02 min

Lab File: BF083556.D

Acq: 7 Dec 2015 11:48

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 410188

Ion Ratio Lower Upper

99 100

42 18.2 17.3 25.9




71 31.0 26.6 40.0

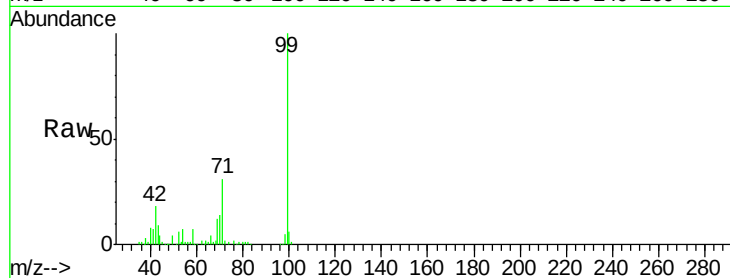

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

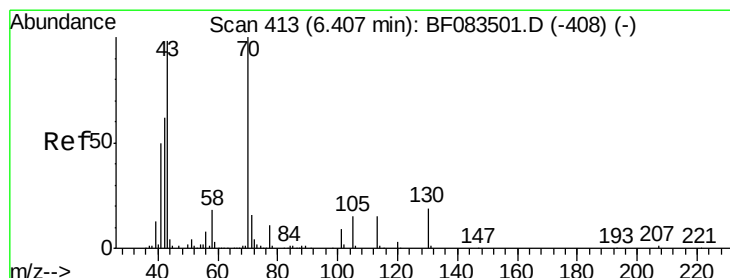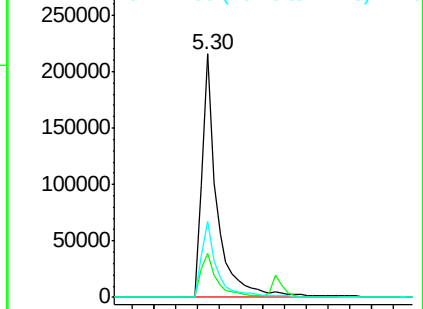

#19

n-Nitroso-di-n-propylamine

Concen: 3.38 ng

RT: 6.56 min Scan# 426

Delta R.T. 0.15 min

Lab File: BF083556.D

Acq: 7 Dec 2015 11:48

Tgt Ion: 70 Resp: 31634


Ion Ratio Lower Upper

70 100

42 52.7 49.2 73.8

101 0.0 7.1 10.7#

130 2.0 15.4 23.0#


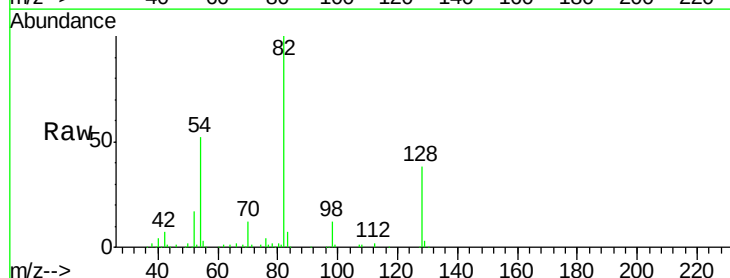





Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0



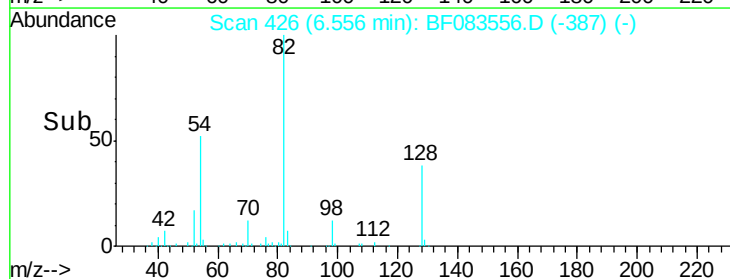
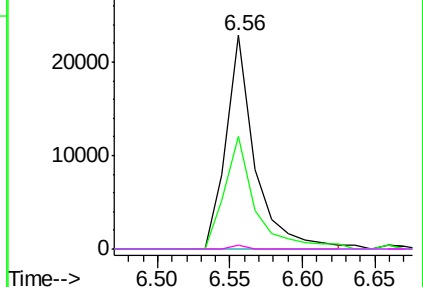


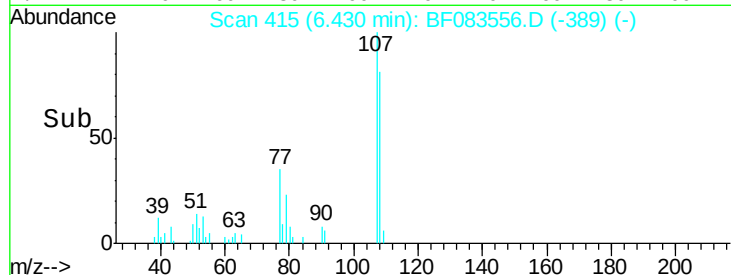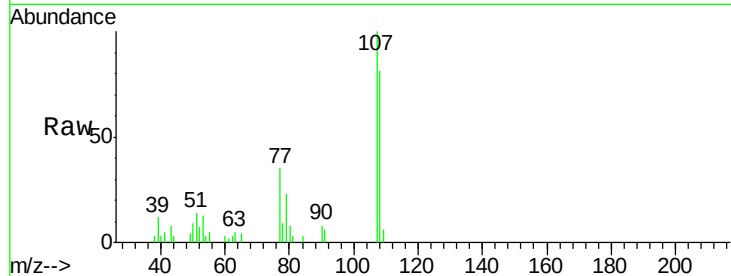

#20
3+4-Methylphenols
Concen: 3.34 ng
RT: 6.43 min Scan# 415
Delta R.T. 0.00 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48


Instrument :
BNA_F
ClientSampleId :


Tot Ion:	107	Resp:	40597
Ion	Ratio	Lower	Upper
107	100		
108	80.9	65.2	105.2
77	34.6	15.2	55.2
79	22.9	6.0	46.0

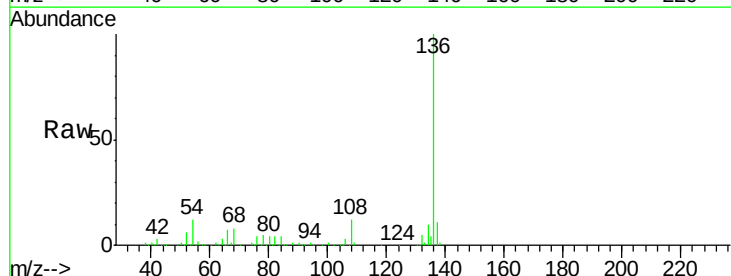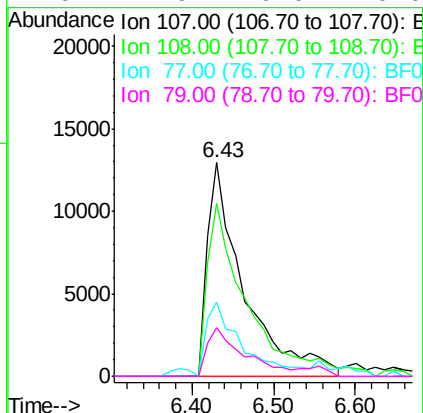

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.63 min Scan# 520
Delta R.T. -0.05 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48

Tgt Ion:	136	Resp:	568449
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.7	13.1
54	12.0	7.8	11.6
68	8.2	5.7	8.5




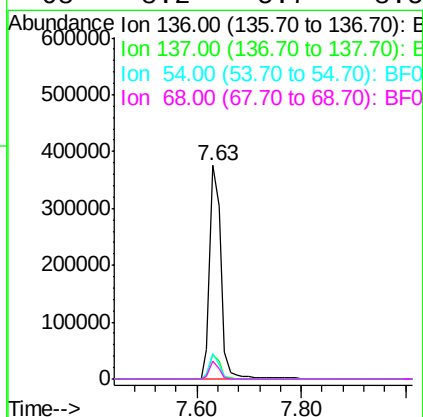




#23
 Nitrobenzene-d5
 Concen: 20.94 ng
 RT: 6.56 min Scan# 426
 Delta R.T. -0.05 min
 Lab File: BF083556.D
 Acq: 7 Dec 2015 11:48




Instrument :
 BNA_F
 ClientSampled :


Tot Ion	82	Resp	254696
Ion Ratio	Lower	Upper	
82	100		
128	38.5	30.7	46.1
54	51.5	42.5	63.7

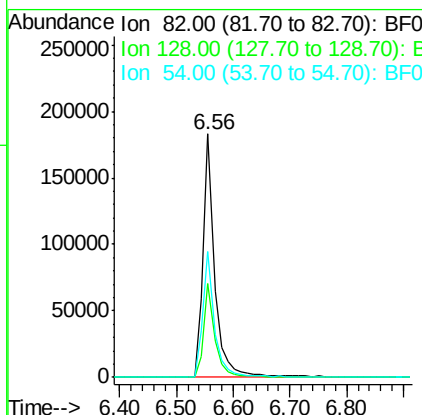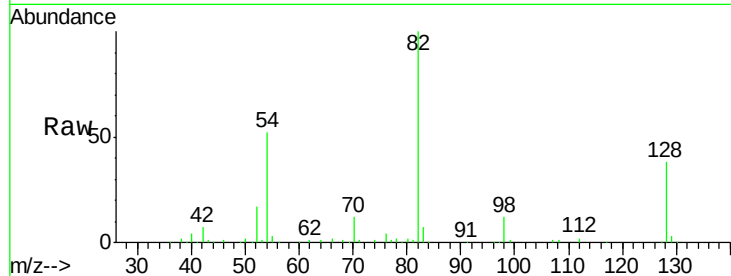

#31
 Naphthalene
 Concen: 2.03 ng
 RT: 7.66 min Scan# 523
 Delta R.T. -0.05 min
 Lab File: BF083556.D
 Acq: 7 Dec 2015 11:48

Tgt Ion	128	Resp	61385
Ion Ratio	Lower	Upper	
128	100		
129	10.8	8.6	13.0
127	13.2	10.6	16.0

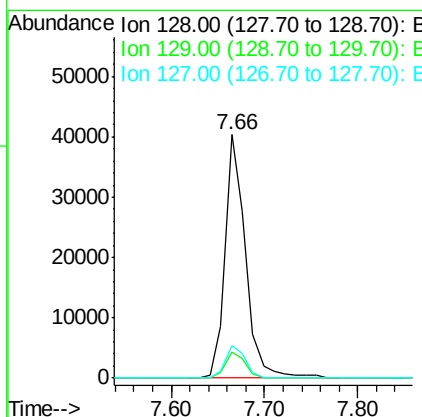







#32
Benzoic acid
Concen: 2.97 ng
RT: 7.46 min Scan# 505
Delta R.T. -0.03 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48

Instrument :
BNA_F
ClientSampleId :

Tot Ion:122 Resp: 1740
Ion Ratio Lower Upper
122 100
105 0.0 105.6 145.6#
77 78.9 86.8 126.8#

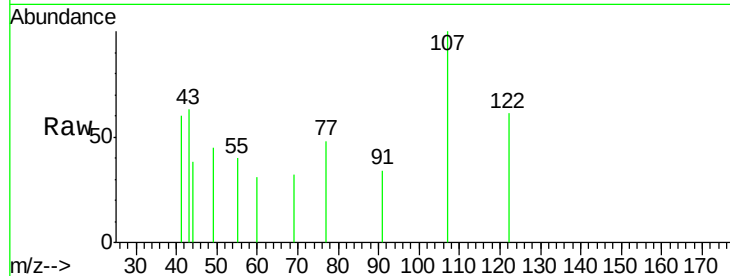


Abundance Ion 122.00 (121.70 to 122.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 77.00 (76.70 to 77.70): BF0

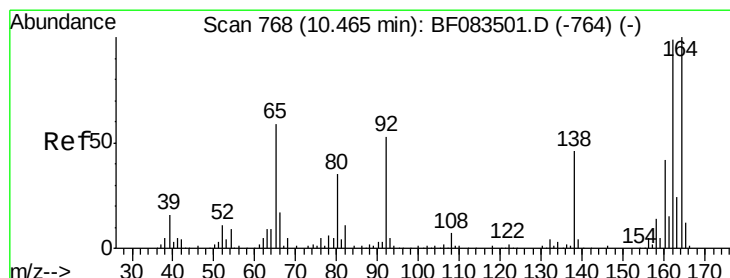
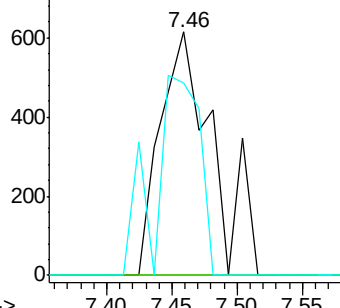



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 10.42 min Scan# 764
Delta R.T. -0.05 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48

Tgt Ion:164 Resp: 262026
Ion Ratio Lower Upper
164 100
162 99.5 78.8 118.2
160 41.9 33.4 50.2

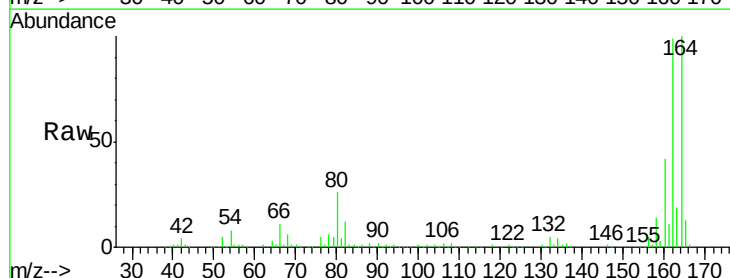

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

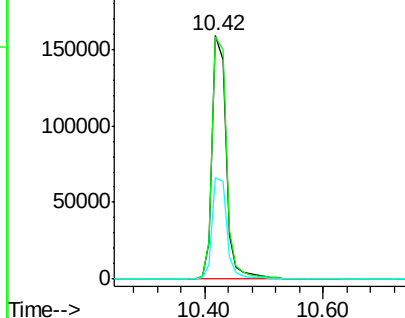







#41
 2,4,6-Tribromophenol
 Concen: 23.59 ng
 RT: 11.71 min Scan# 877
 Delta R.T. -0.05 min
 Lab File: BF083556.D
 Acq: 7 Dec 2015 11:48

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 57026
 Ion Ratio Lower Upper
 330 100
 332 96.9 0.0 0.0#
 141 42.1 0.0 0.0#

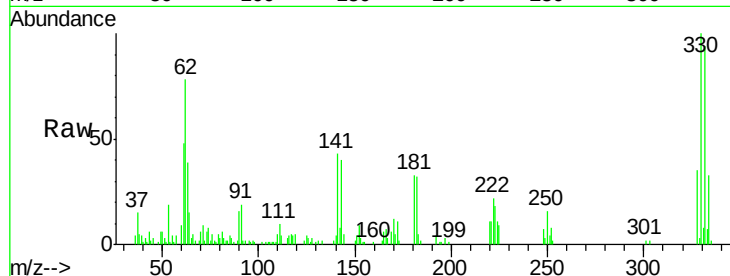


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

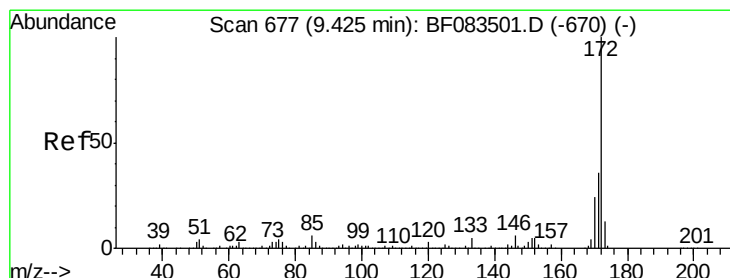
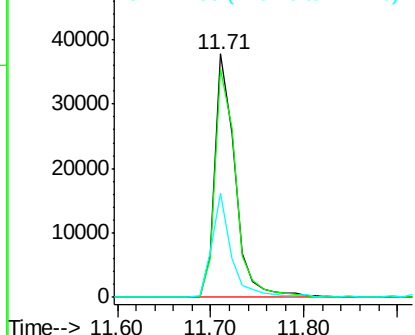



#44
 2-Fluorobiphenyl
 Concen: 19.37 ng
 RT: 9.38 min Scan# 673
 Delta R.T. -0.05 min
 Lab File: BF083556.D
 Acq: 7 Dec 2015 11:48

Tgt Ion:172 Resp: 374184
 Ion Ratio Lower Upper
 172 100
 171 34.6 28.6 42.8
 170 22.5 19.4 29.0

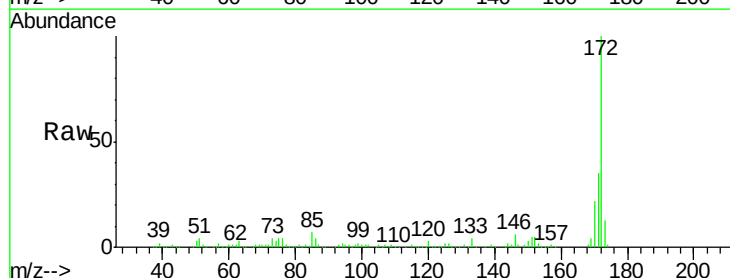

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

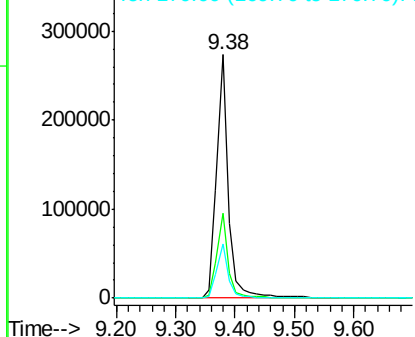



#49

Dimethylphthalate

Concen: 3.94 ng

RT: 10.06 min Scan# 733

Delta R.T. -0.05 min

Lab File: BF083556.D

Acq: 7 Dec 2015 11:48

Instrument :

BNA_F

ClientSampleId :


Tot Ion:163 Resp: 81208

Ion Ratio Lower Upper

163 100

194 2.8 2.8 4.2#




164 10.3 8.6 13.0



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

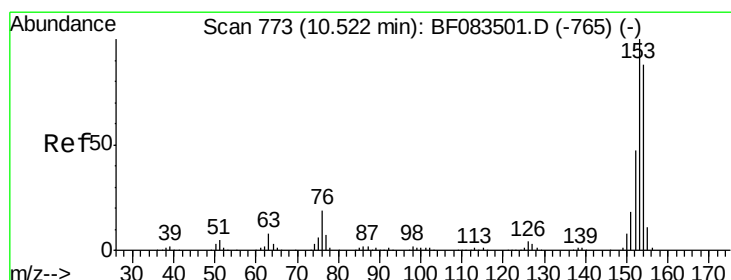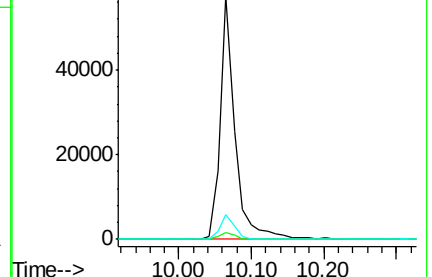

#51

Acenaphthene

Concen: 3.72 ng

RT: 10.48 min Scan# 769

Delta R.T. -0.05 min

Lab File: BF083556.D

Acq: 7 Dec 2015 11:48


Tgt Ion:154 Resp: 61549

Ion Ratio Lower Upper

154 100

153 111.7 91.4 137.0



152 56.5 43.4 65.2




Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E



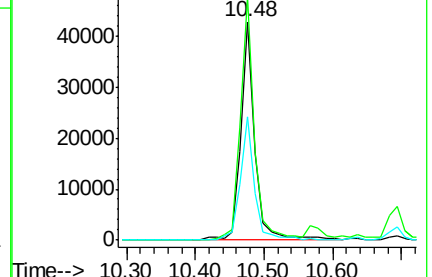





#54
Dibenzenofuran
Concen: 2.13 ng
RT: 10.76 min Scan# 794
Delta R.T. -0.05 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48




Instrument :
BNA_F
ClientSampleId :


Tot Ion:168 Resp: 48733
Ion Ratio Lower Upper
168 100
139 38.3 28.0 42.0
169 14.9 10.8 16.2

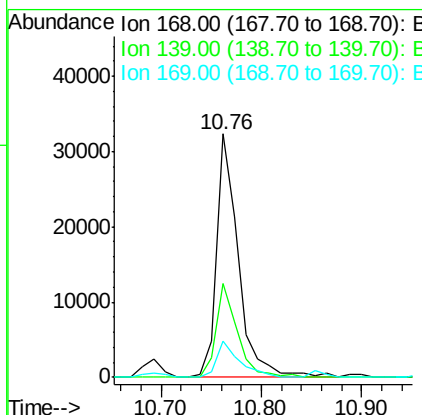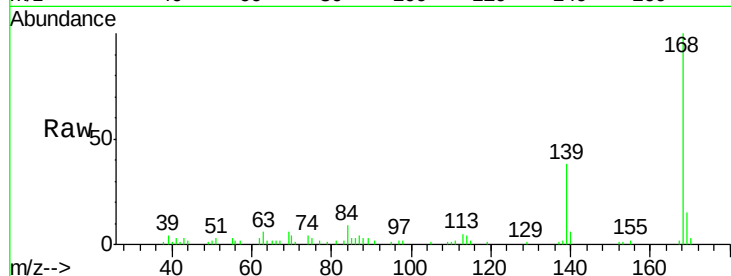

#55
4-Nitrophenol
Concen: 7.04 ng
RT: 10.76 min Scan# 794
Delta R.T. -0.07 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48

Tgt Ion:139 Resp: 18574
Ion Ratio Lower Upper
139 100
109 2.9 42.0 82.0#
65 4.9 89.2 129.2#

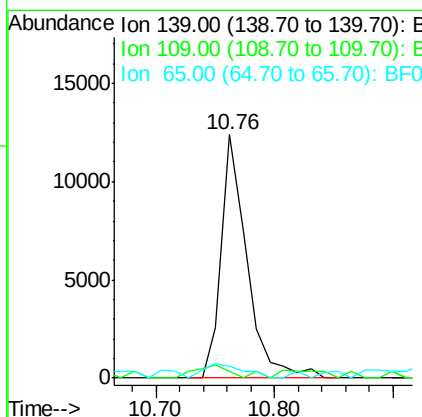

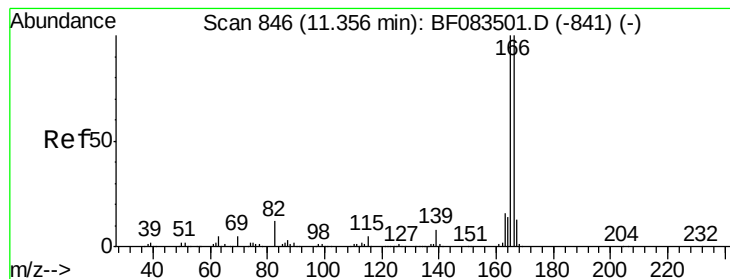

#57

Fluorene

Concen: 3.39 ng

RT: 11.31 min Scan# 842

Delta R.T. -0.05 min

Lab File: BF083556.D

Acq: 7 Dec 2015 11:48

Instrument :

BNA_F

ClientSampleId :


Tot Ion:166 Resp: 67561

Ion Ratio Lower Upper

166 100

165 103.0 80.0 120.0




167 13.3 10.6 16.0

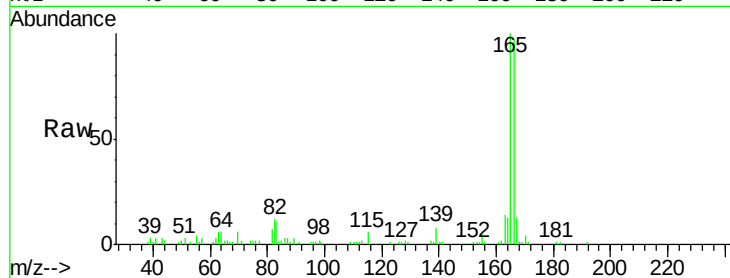

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

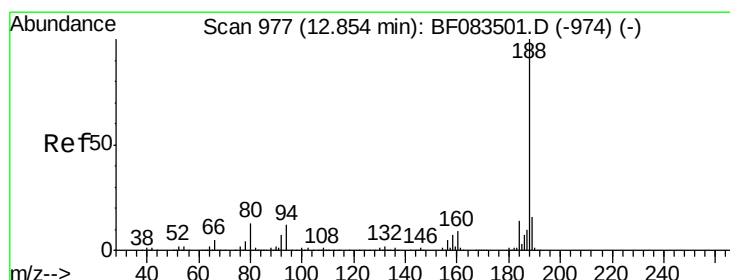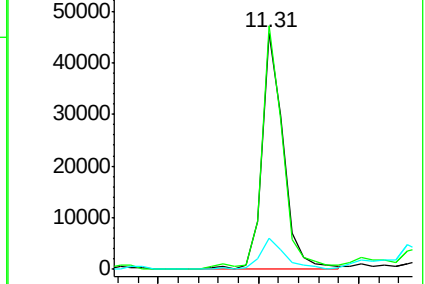

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 12.82 min Scan# 974

Delta R.T. -0.03 min

Lab File: BF083556.D

Acq: 7 Dec 2015 11:48


Tgt Ion:188 Resp: 403025

Ion Ratio Lower Upper

188 100

94 10.7 9.4 14.2



80 12.6 10.6 16.0

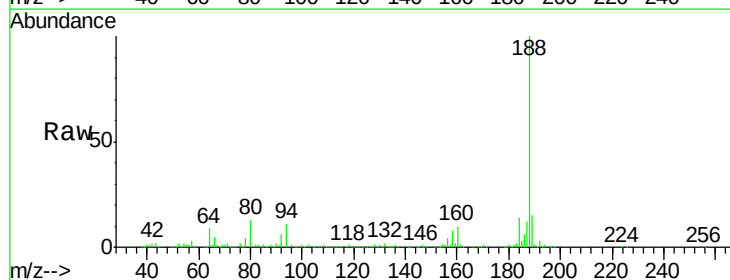


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



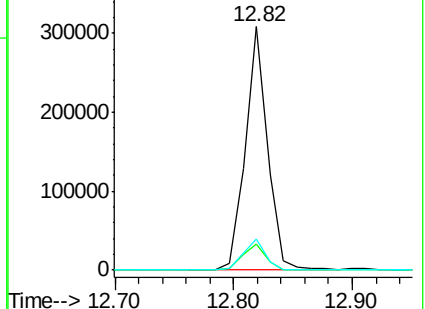





#70
Phenanthrene
Concen: 28.01 ng
RT: 12.85 min Scan# 977
Delta R.T. -0.05 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48




Instrument :
BNA_F
ClientSampleId :


Tot Ion:178 Resp: 657099
Ion Ratio Lower Upper
178 100
176 19.6 15.7 23.5
179 15.8 12.2 18.4

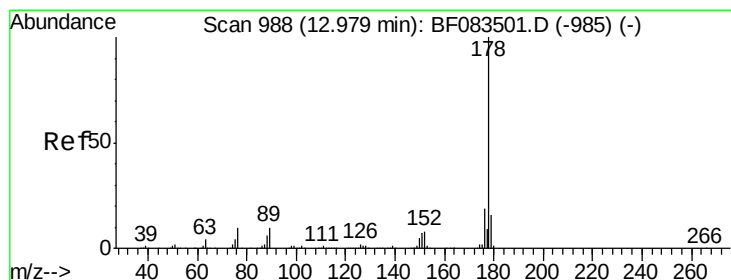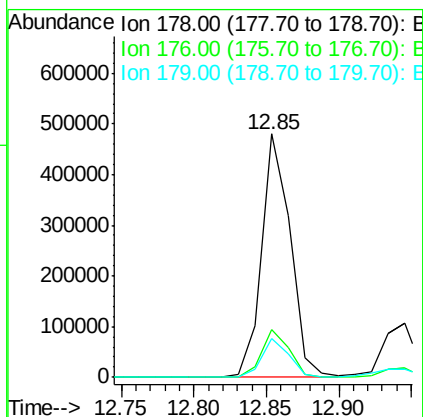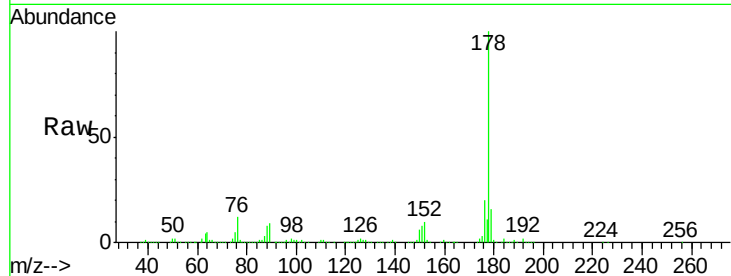

#71
Anthracene
Concen: 6.65 ng
RT: 12.95 min Scan# 985
Delta R.T. -0.03 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48

Tgt Ion:178 Resp: 159061
Ion Ratio Lower Upper
178 100
176 16.7 15.2 22.8
179 15.9 12.6 18.8

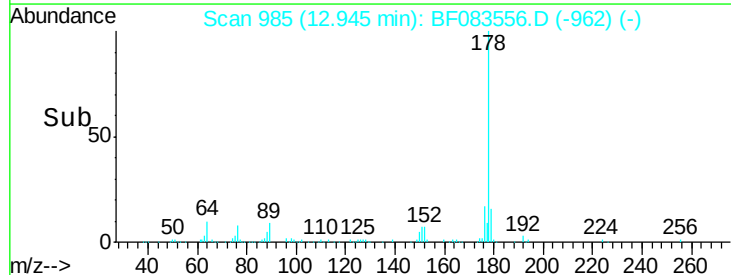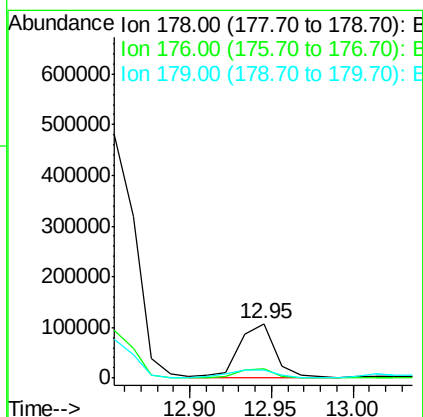



#72

Carbazole

Concen: 2.86 ng

RT: 13.24 min Scan# 1011

Delta R.T. -0.03 min

Lab File: BF083556.D

Acq: 7 Dec 2015 11:48

Instrument :

BNA_F

ClientSampleId :


Tot Ion:167 Resp: 58674

Ion Ratio Lower Upper

167 100

166 20.9 17.2 25.8




139 13.1 9.3 13.9



Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

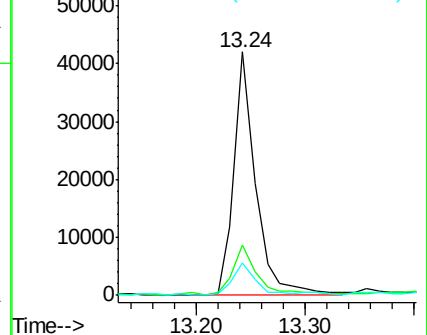

#74

Fluoranthene

Concen: 30.88 ng

RT: 14.79 min Scan# 1146

Delta R.T. -0.03 min

Lab File: BF083556.D

Acq: 7 Dec 2015 11:48


Tgt Ion:202 Resp: 717946

Ion Ratio Lower Upper

202 100

101 13.0 0.0 31.5



203 18.0 0.0 37.6




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

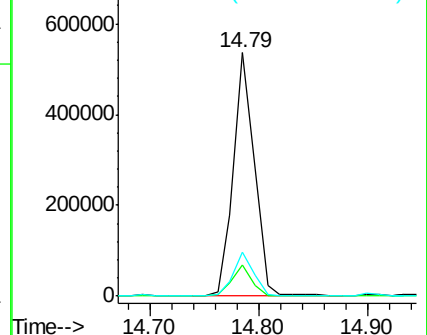



#75

Chrysene-d12

Concen: 20.00 ng

RT: 17.01 min Scan# 1341

Delta R.T. -0.03 min

Lab File: BF083556.D

Acq: 7 Dec 2015 11:48

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 340409

Ion Ratio Lower Upper

240 100

120 13.6 8.1 12.1#




236 25.2 20.8 31.2



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

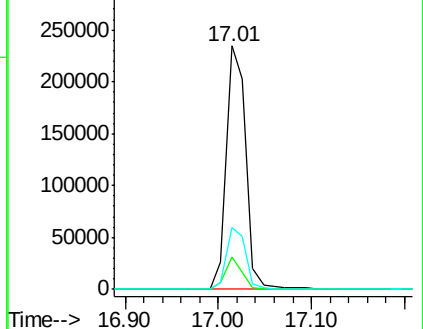

#77

Pyrene

Concen: 24.24 ng

RT: 15.14 min Scan# 1177

Delta R.T. -0.03 min

Lab File: BF083556.D

Acq: 7 Dec 2015 11:48


Tgt Ion:202 Resp: 617385

Ion Ratio Lower Upper

202 100

200 20.6 16.7 25.1



203 22.3 14.3 21.5#




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E




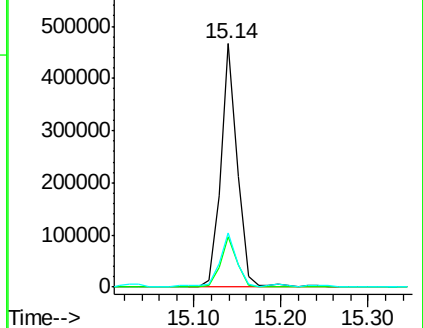




#78
 Terphenyl-d14
 Concen: 16.02 ng
 RT: 15.45 min Scan# 1204
 Delta R.T. -0.03 min
 Lab File: BF083556.D
 Acq: 7 Dec 2015 11:48




Instrument :
 BNA_F
 ClientSampled :


Tot Ion:244 Resp: 245132
 Ion Ratio Lower Upper
 244 100
 212 7.3 6.1 9.1
 122 11.1 11.0 16.6

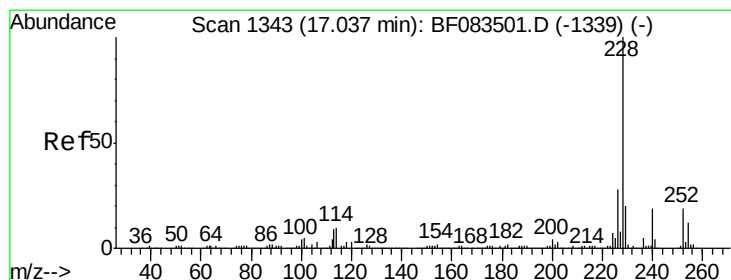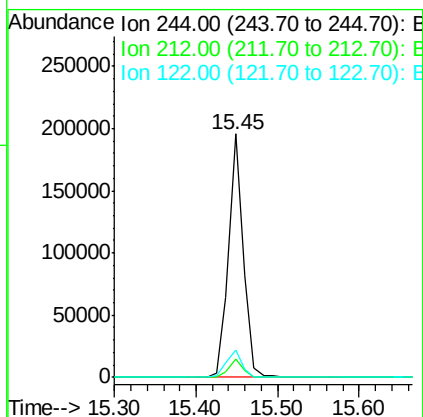

#80
 Benzo(a)anthracene
 Concen: 14.56 ng
 RT: 17.00 min Scan# 1340
 Delta R.T. -0.03 min
 Lab File: BF083556.D
 Acq: 7 Dec 2015 11:48

Tgt Ion:228 Resp: 290042
 Ion Ratio Lower Upper
 228 100
 226 27.7 22.3 33.5
 229 22.3 15.7 23.5



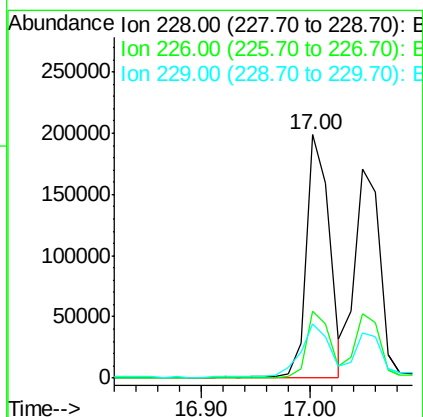
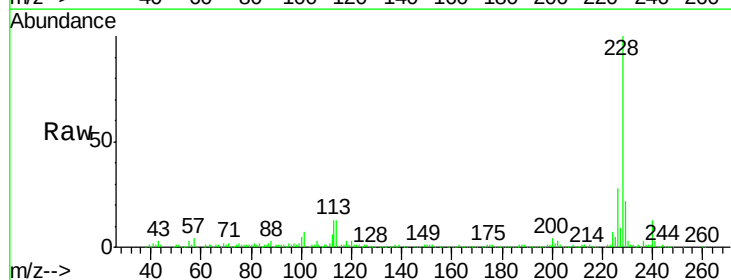




#82
Chrysene
Concen: 13.84 ng
RT: 17.05 min Scan# 1344
Delta R.T. -0.03 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48




Instrument :
BNA_F
ClientSampleId :


Tot Ion:228 Resp: 274622
Ion Ratio Lower Upper
228 100
226 30.9 24.7 37.1
229 21.5 16.3 24.5

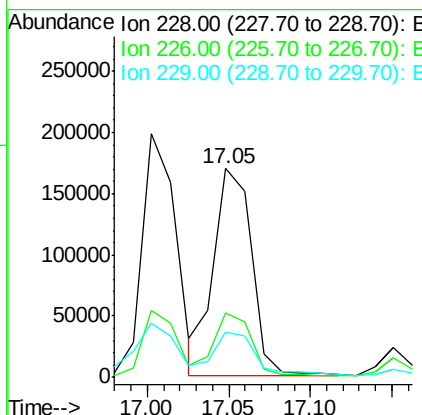

#85
Indeno(1,2,3-cd)pyrene
Concen: 4.96 ng
RT: 19.89 min Scan# 1593
Delta R.T. -0.02 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48

Tgt Ion:276 Resp: 84284
Ion Ratio Lower Upper
276 100
138 23.9 0.0 0.0#
277 27.1 0.0 0.0#

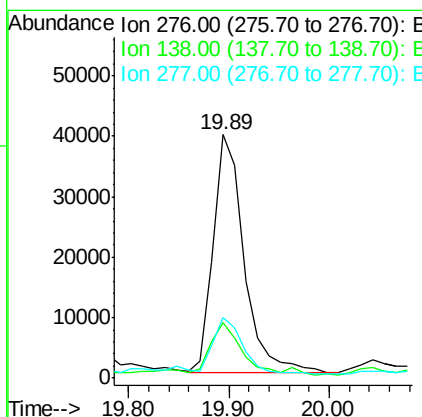







#86
Pervlene-d12
Concen: 20.00 ng
RT: 18.65 min Scan# 1484
Delta R.T. -0.02 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48

Instrument :
BNA_F
ClientSampleId :

Tot Ion:264 Resp: 268777
Ion Ratio Lower Upper
264 100
260 23.7 19.4 29.0
265 22.3 17.8 26.6




Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

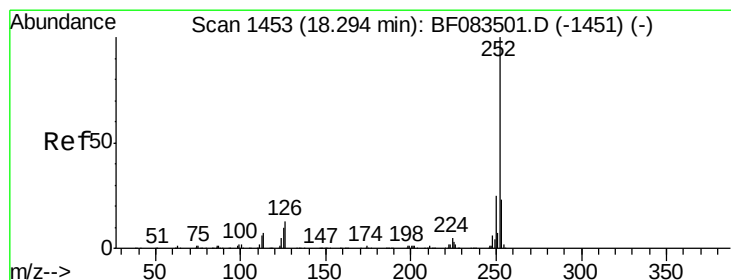
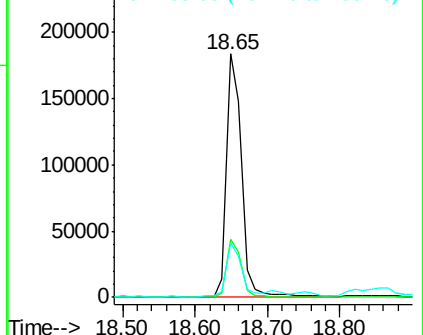



#87
Benzo(b)fluoranthene
Concen: 22.47 ng
RT: 18.27 min Scan# 1451
Delta R.T. -0.02 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48

Tgt Ion:252 Resp: 339199
Ion Ratio Lower Upper
252 100
253 21.9 18.2 27.4
125 13.0 8.2 12.4#

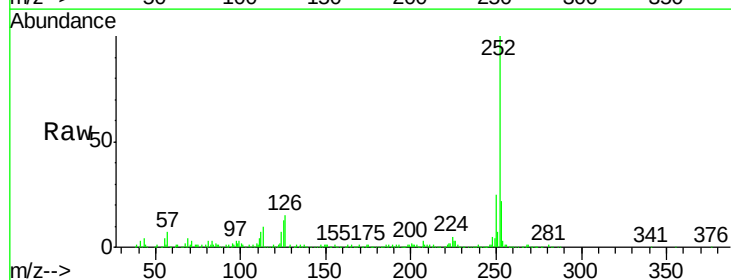

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E




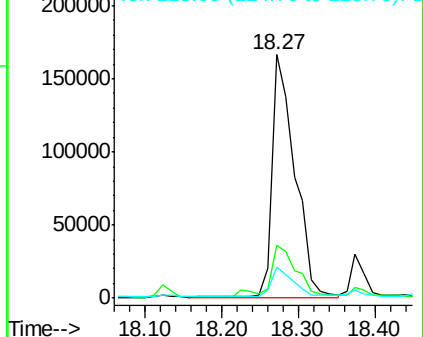




#88
Benzo(k)fluoranthene
Concen: 21.94 ng
RT: 18.27 min Scan# 1451
Delta R.T. -0.05 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48




Instrument :
BNA_F
ClientSampleId :


Tot Ion:252 Resp: 339199
Ion Ratio Lower Upper
252 100
253 21.9 18.6 27.8
125 13.0 11.5 17.3

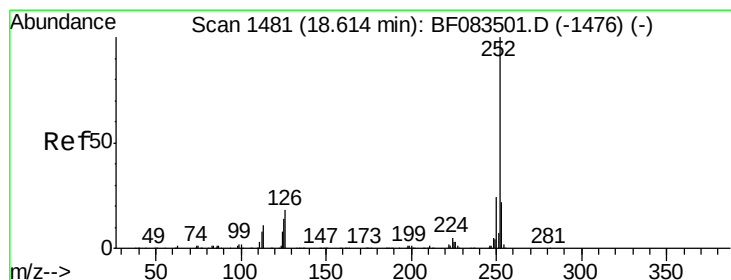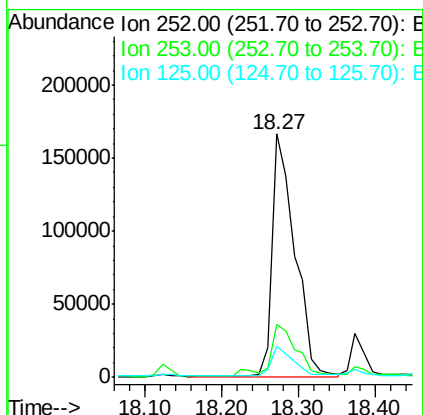

#89
Benzo(a)pyrene
Concen: 8.09 ng
RT: 18.55 min Scan# 1475
Delta R.T. -0.07 min
Lab File: BF083556.D
Acq: 7 Dec 2015 11:48

Tgt Ion:252 Resp: 118752
Ion Ratio Lower Upper
252 100
253 23.9 17.5 26.3
125 14.2 11.0 16.6

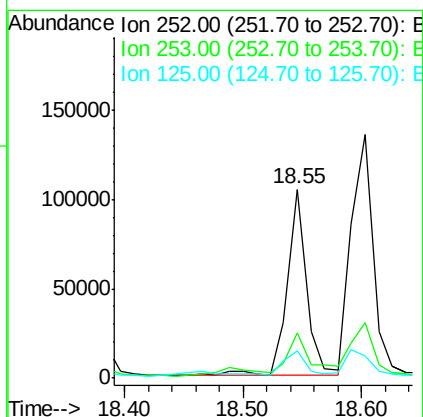



#91
 Benzo(a,h,i)perylene
 Concen: 5.69 ng
 RT: 20.26 min Scan# 1625
 Delta R.T. -0.01 min
 Lab File: BF083556.D
 Acq: 7 Dec 2015 11:48

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
276	100		
277	24.8	19.2	28.8
138	22.9	19.5	29.3

