
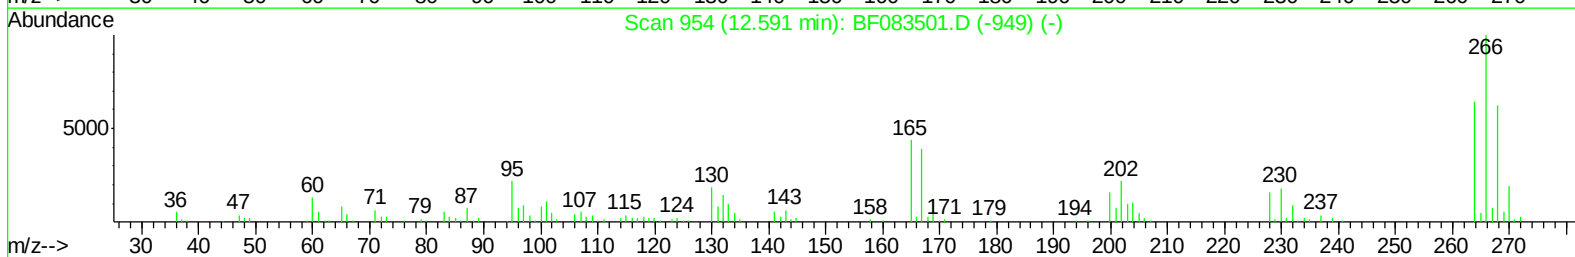
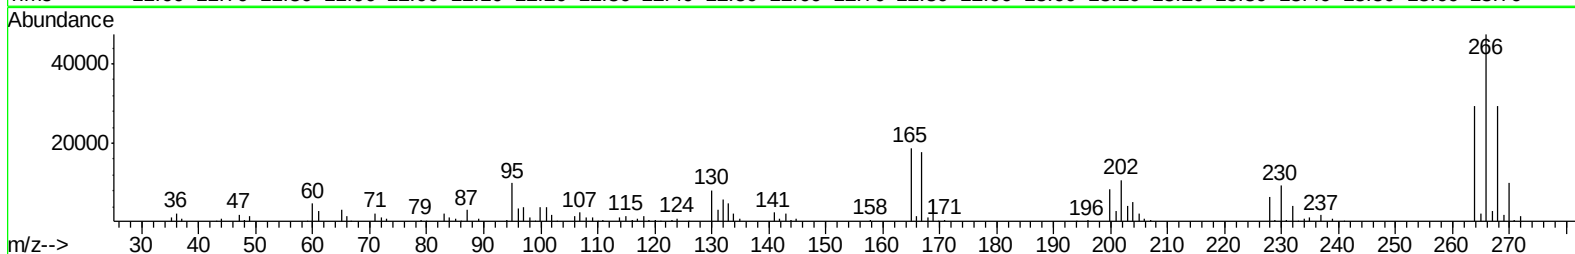


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120615\
Data File : BF083525.D
Acq On : 6 Dec 2015 12:24
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 08:53:45 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 05 04:12:46 2015
Response via : Initial Calibration

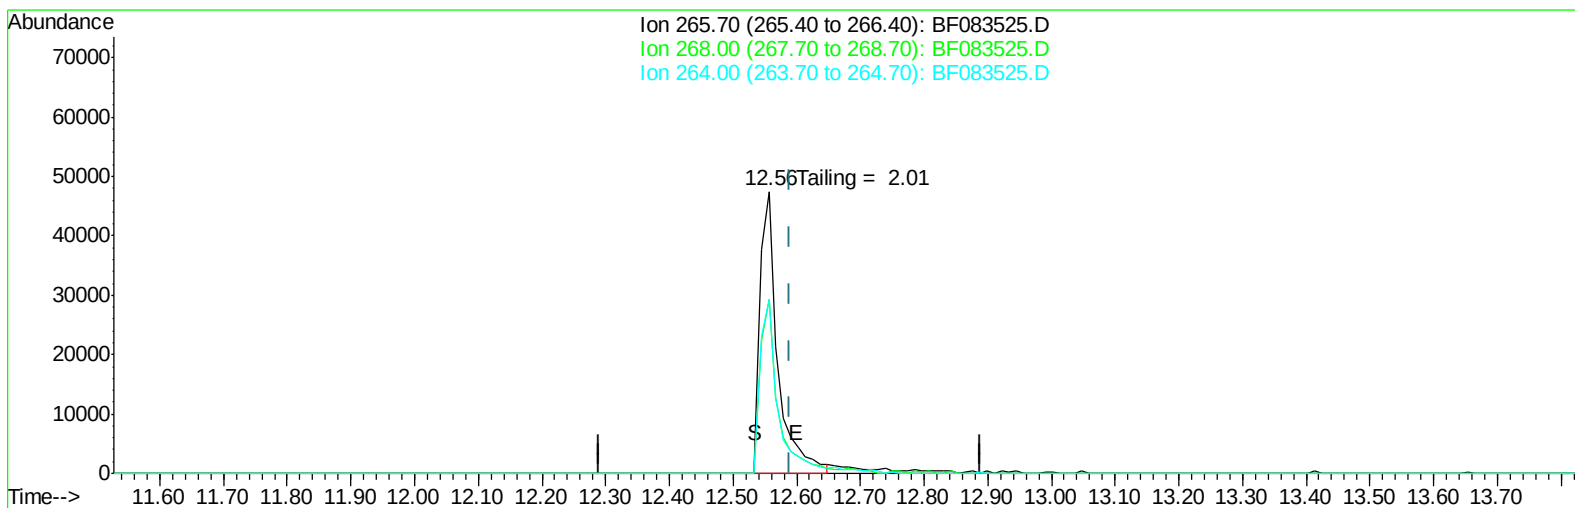

TIC: BF083525.D

(69) Pentachlorophenol (C)




12.556min (-0.034) 0.00ng

response 99382

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	62.04
264.00	64.30	61.92
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF120615\
Data File : BF083534.D
Acq On : 7 Dec 2015 00:02
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 09:04:46 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 05 04:12:46 2015
Response via : Initial Calibration

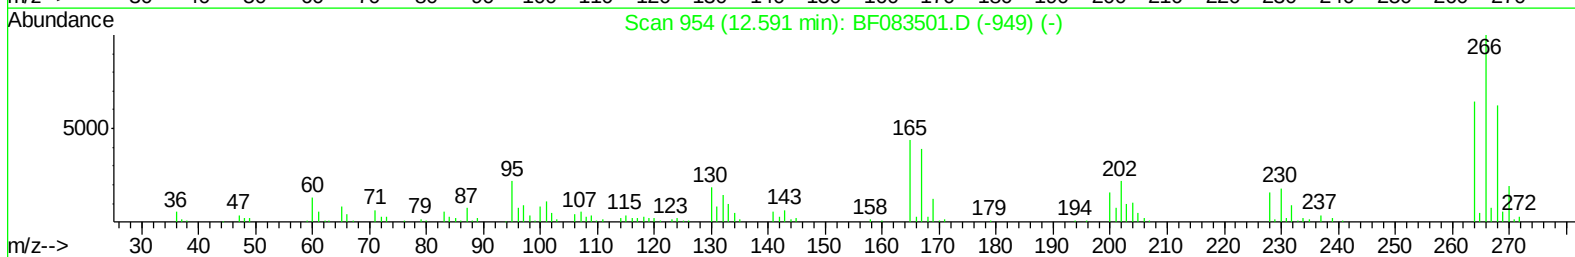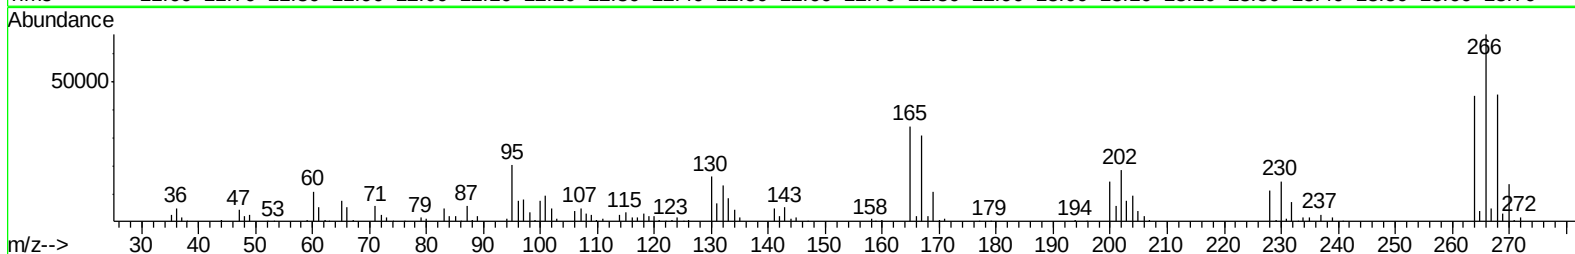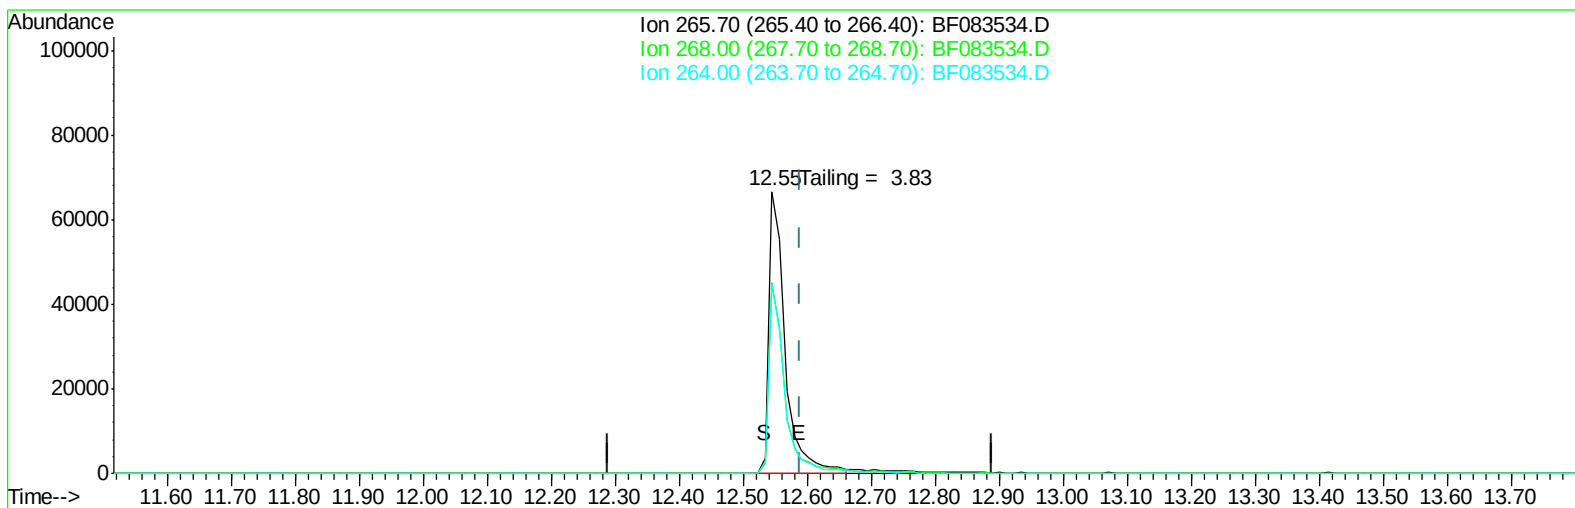

TIC: BF083534.D

(69) Pentachlorophenol (C)

12.545min (-0.045) 45223.24ng m

response 117455

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	67.86
264.00	64.30	67.48
0.00	0.00	0.00