


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120615\
Data File : BF083525.D
Acq On : 6 Dec 2015 12:24
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Dec 05 04:12:46 2015

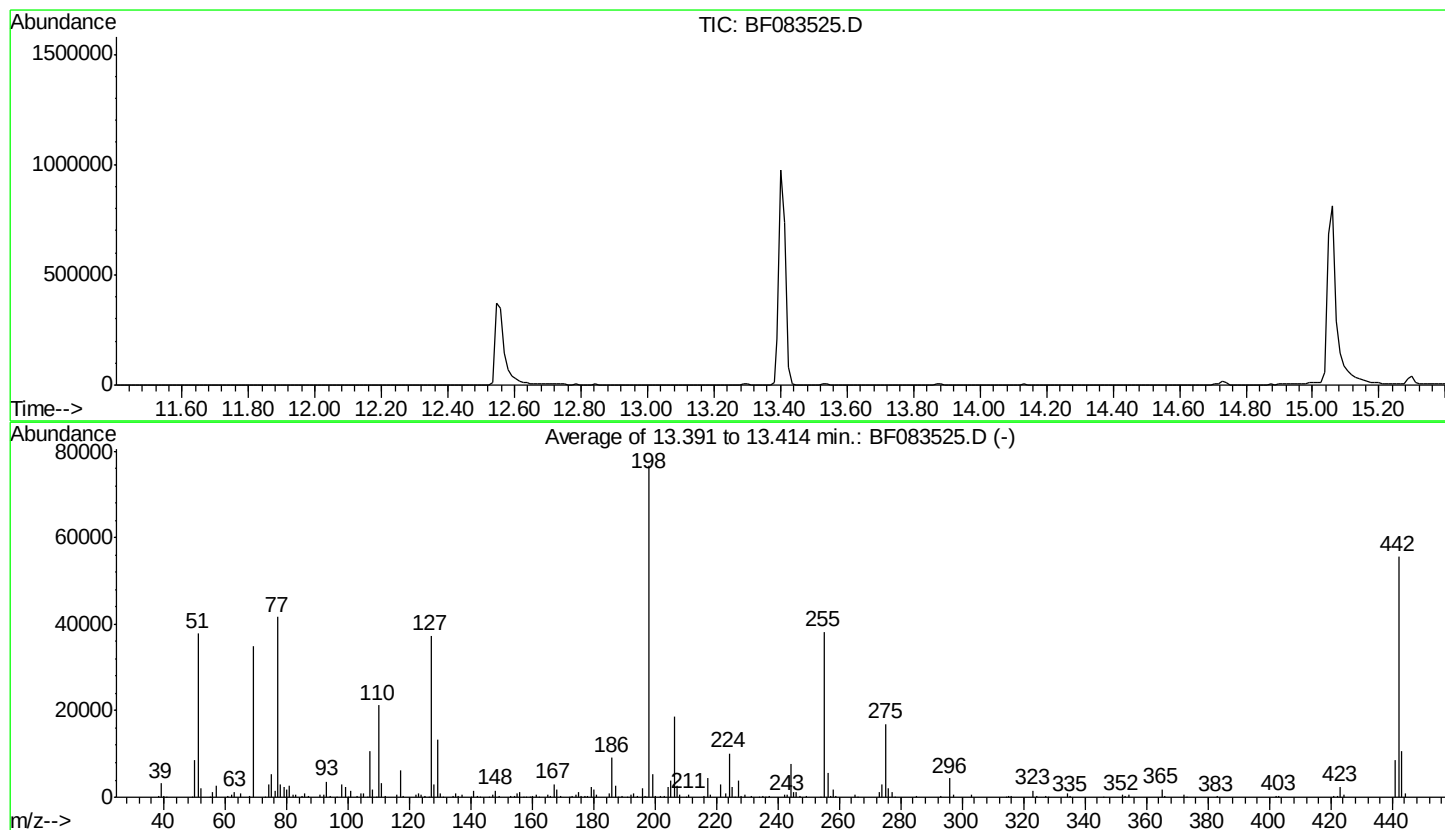

AutoFind: Scans 1024, 1025, 1026; Background Corrected with Scan 1020

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.4	37882	PASS
68	69	0.00	2	1.1	382	PASS
69	198	0.00	100	45.6	34997	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	37376	PASS
197	198	0.00	2	0.3	242	PASS
198	198	100	100	100.0	76669	PASS
199	198	5	9	7.1	5425	PASS
275	198	10	60	22.1	16953	PASS
365	198	1	100	2.4	1849	PASS
441	442	0.01	24	15.6	8642	PASS
442	198	50	100	72.4	55525	PASS
443	442	15	24	19.2	10682	PASS