


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120615\
Data File : BF083534.D
Acq On : 7 Dec 2015 00:02
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Dec 05 04:12:46 2015

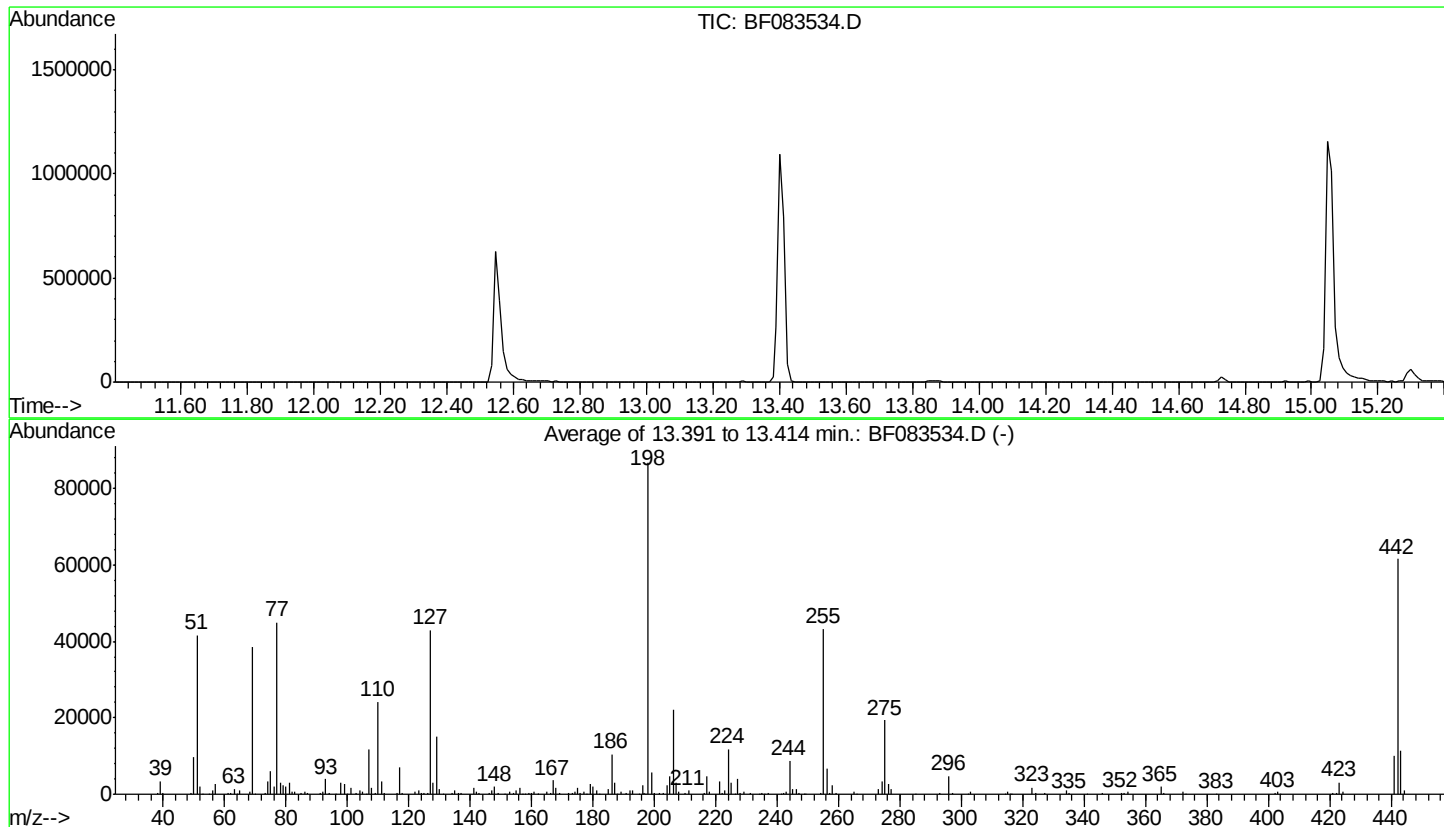

AutoFind: Scans 1024, 1025, 1026; Background Corrected with Scan 1020

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.9	41562	PASS
68	69	0.00	2	1.6	596	PASS
69	198	0.00	100	44.3	38424	PASS
70	69	0.00	2	0.3	108	PASS
127	198	10	80	49.6	43016	PASS
197	198	0.00	2	0.3	288	PASS
198	198	100	100	100.0	86760	PASS
199	198	5	9	6.8	5859	PASS
275	198	10	60	22.4	19404	PASS
365	198	1	100	2.3	1963	PASS
441	442	0.01	24	16.3	10035	PASS
442	198	50	100	70.9	61499	PASS
443	442	15	24	18.3	11263	PASS