
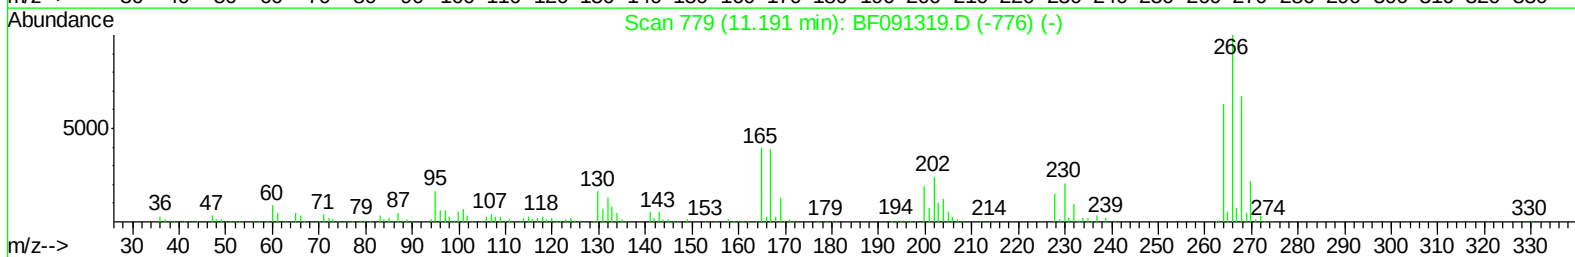
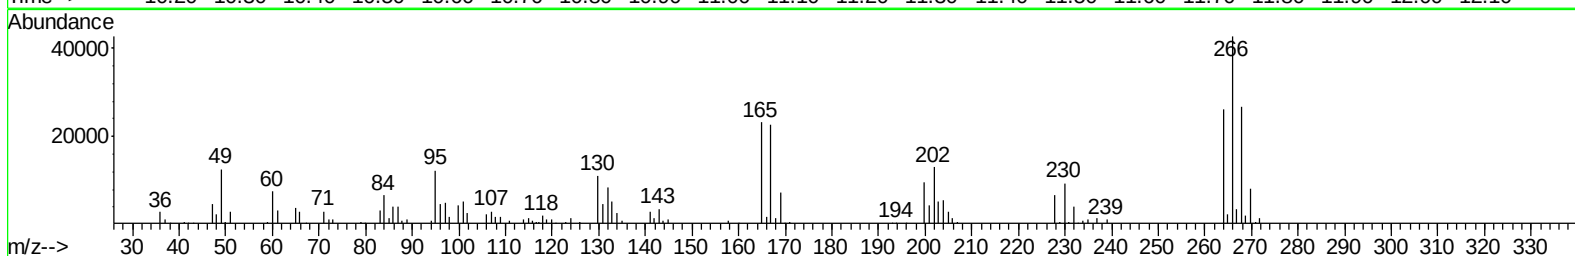


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120616\
Data File : BF091449.D
Acq On : 6 Dec 2016 10:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 01:17:13 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 00:12:14 2016
Response via : Initial Calibration

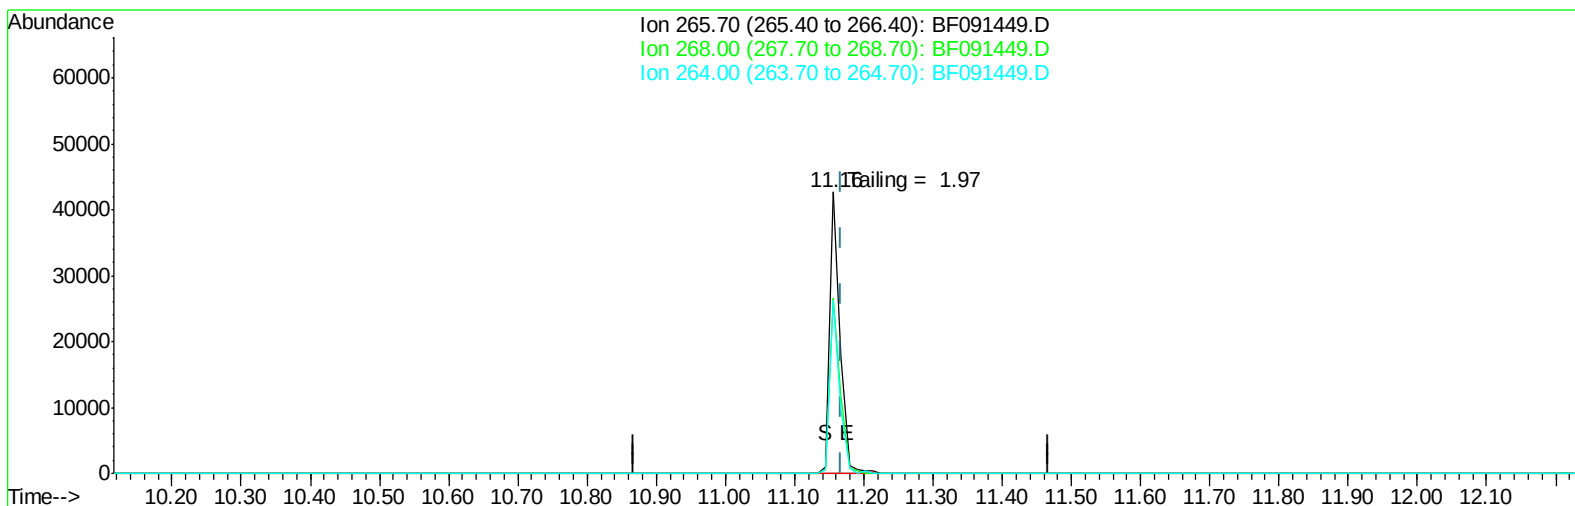

TIC: BF091449.D

(69) Pentachlorophenol (C)




11.156min (-0.012) 0.00ng

response 43888

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	62.49
264.00	60.20	61.22
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF120616\
 Data File : BF091449.D
 Acq On : 6 Dec 2016 10:37
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 01:17:13 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 07 00:12:14 2016
 Response via : Initial Calibration

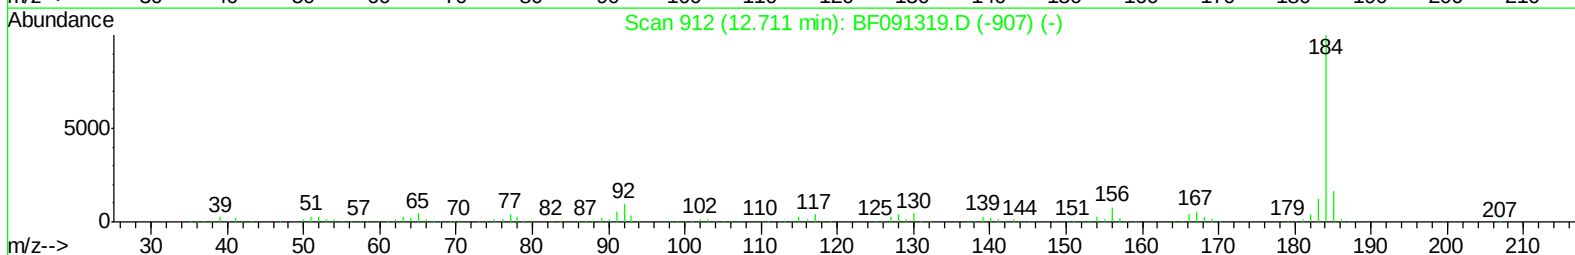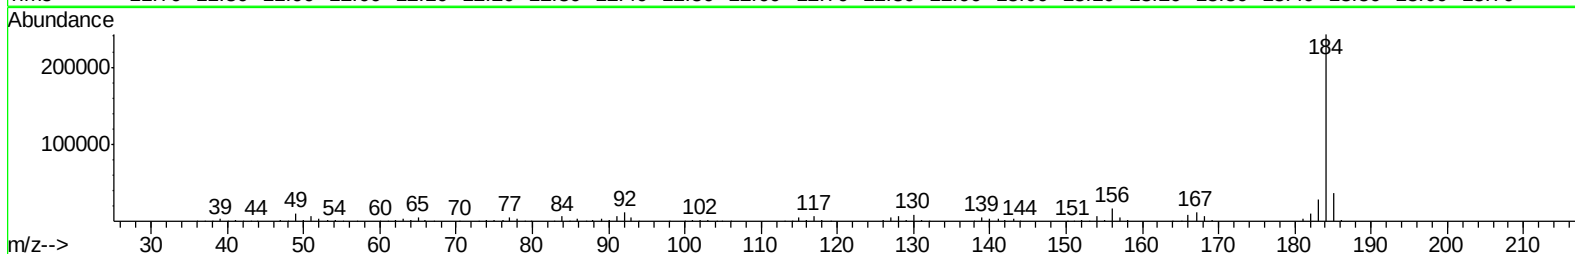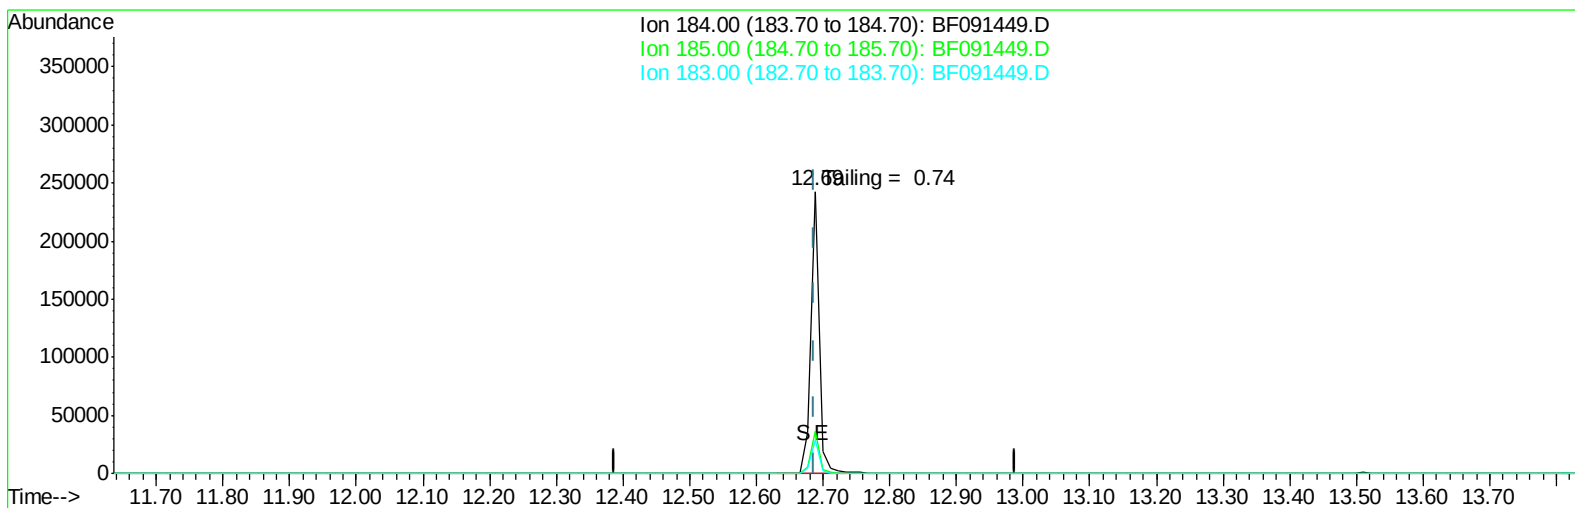

TIC: BF091449.D

(76) Benzidine

12.688min (-0.000) 0.00ng

response 211955

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	15.14
183.00	11.10	11.85
0.00	0.00	0.00