


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120616\
 Data File : BF091449.D
 Acq On : 6 Dec 2016 10:37
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 13:33:46 2016

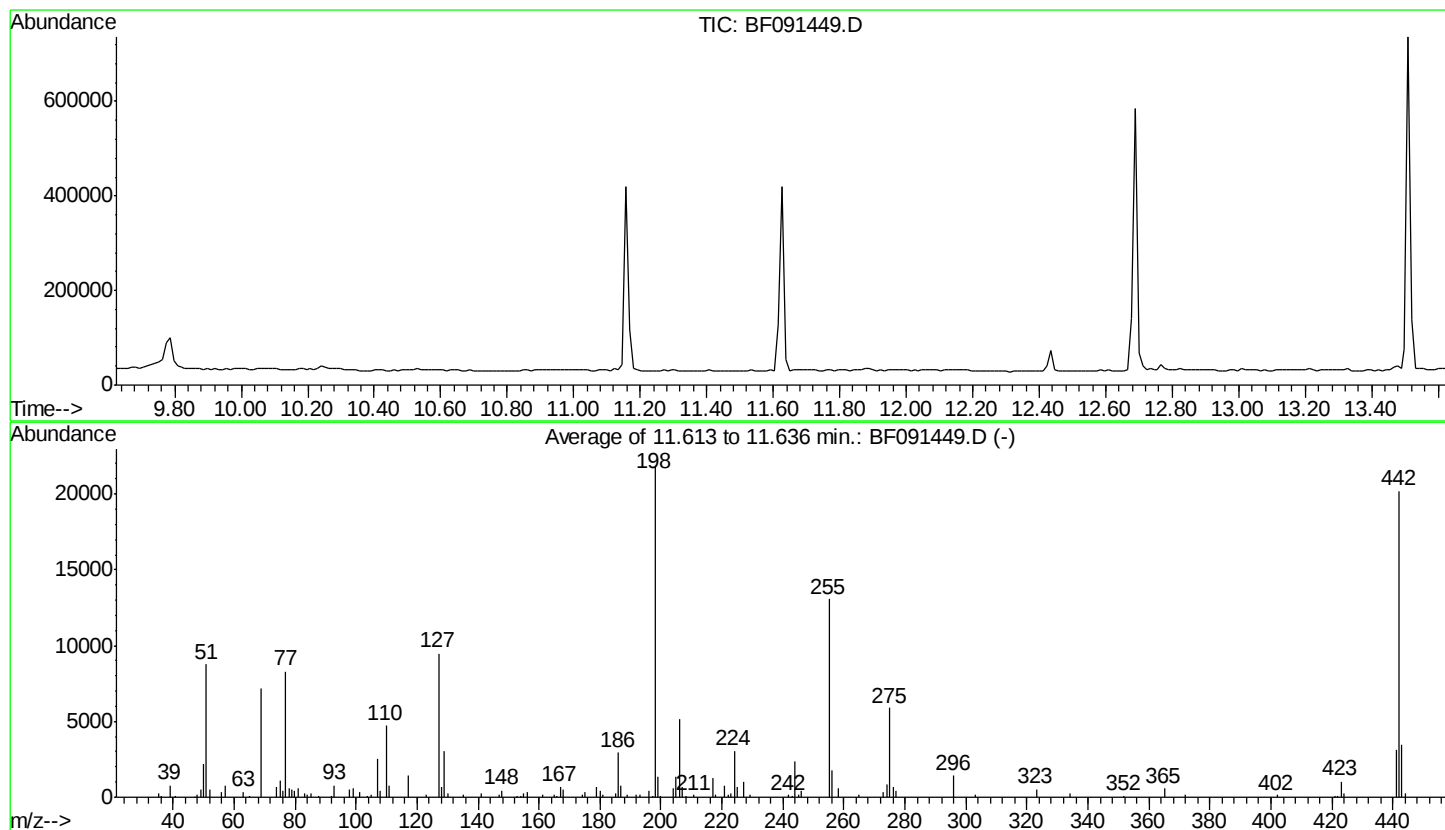

AutoFind: Scans 816, 817, 818; Background Corrected with Scan 813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	8767	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.7	7150	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.3	9468	PASS
197	198	0.00	2	0.6	125	PASS
198	198	100	100	100.0	21871	PASS
199	198	5	9	6.3	1369	PASS
275	198	10	60	26.8	5872	PASS
365	198	1	100	2.6	571	PASS
441	442	0.01	24	15.3	3092	PASS
442	198	50	100	92.4	20219	PASS
443	442	15	24	17.3	3489	PASS