
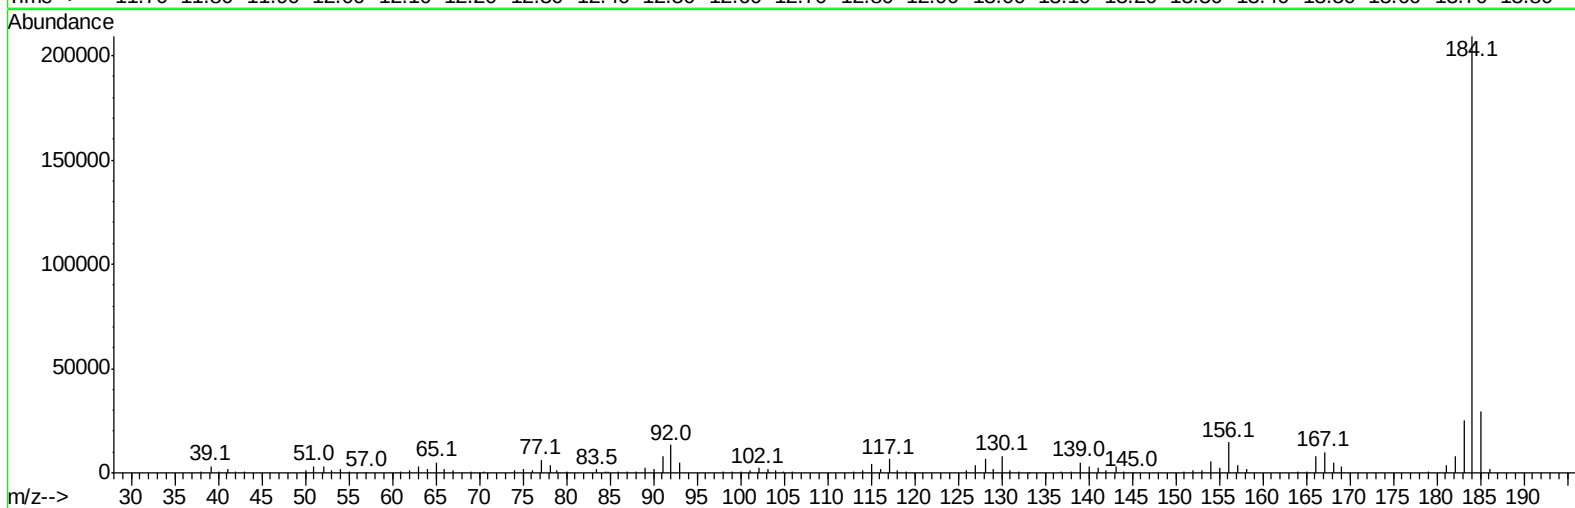


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF120617\
Data File : BF101159.D
Acq On : 6 Dec 2017 11:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:49:09 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:07:49 2017
Response via : Initial Calibration

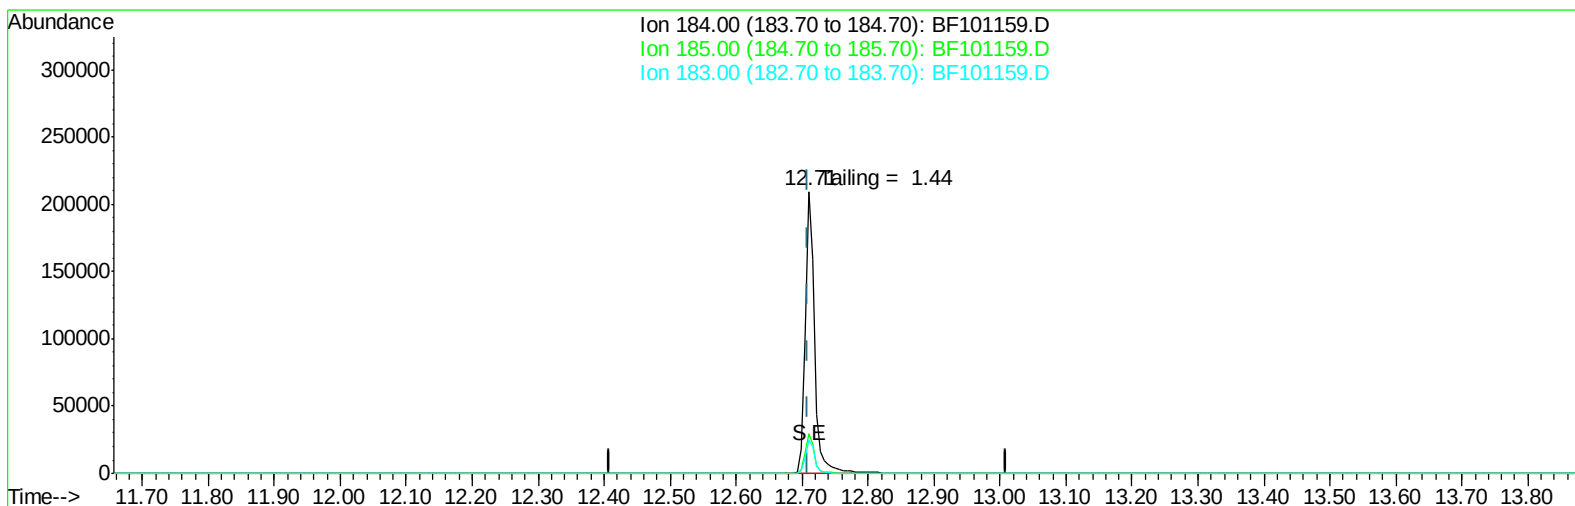

TIC: BF101159.D

(76) Benzidine



12.710min (+0.000) 0.00ng

response 208812

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.22
183.00	11.60	11.99
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF120617\
Data File : BF101159.D
Acq On : 6 Dec 2017 11:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:49:09 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:07:49 2017
Response via : Initial Calibration

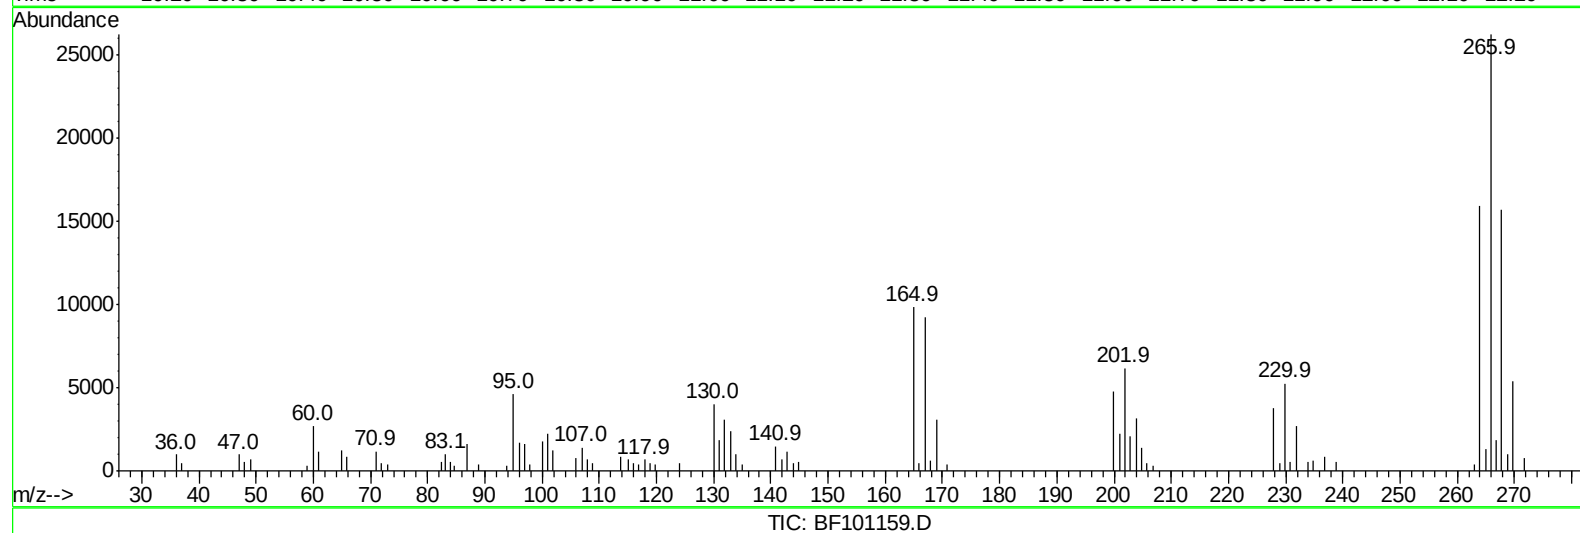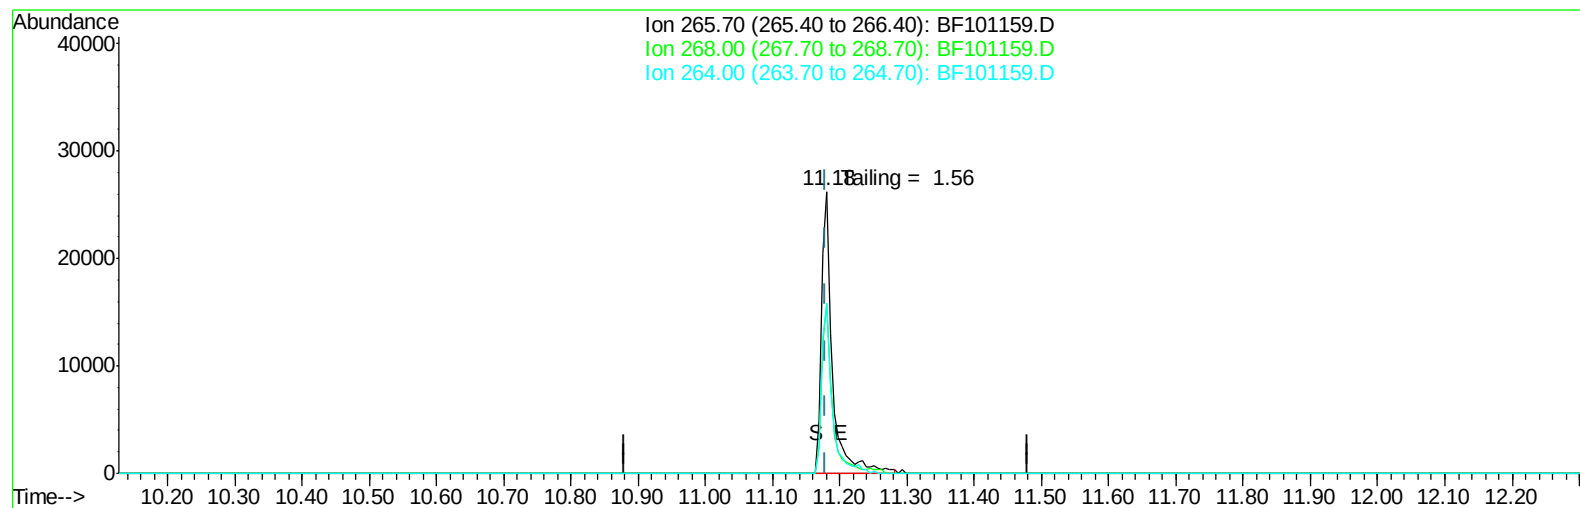

(69) Pentachlorophenol (C)

11.180min (+0.000) 0.00ng

response 30408

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.94
264.00	61.90	60.57
0.00	0.00	0.00