
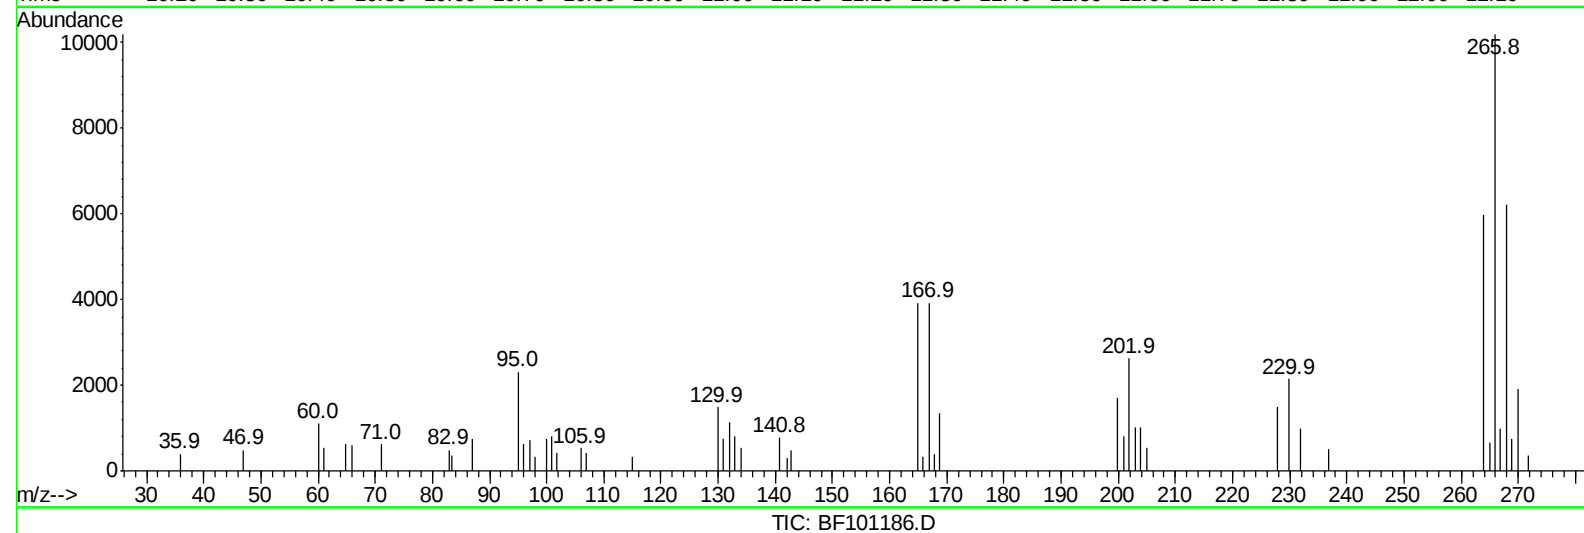


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF120617\
Data File : BF101186.D
Acq On : 7 Dec 2017 00:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:50:34 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:07:49 2017
Response via : Initial Calibration

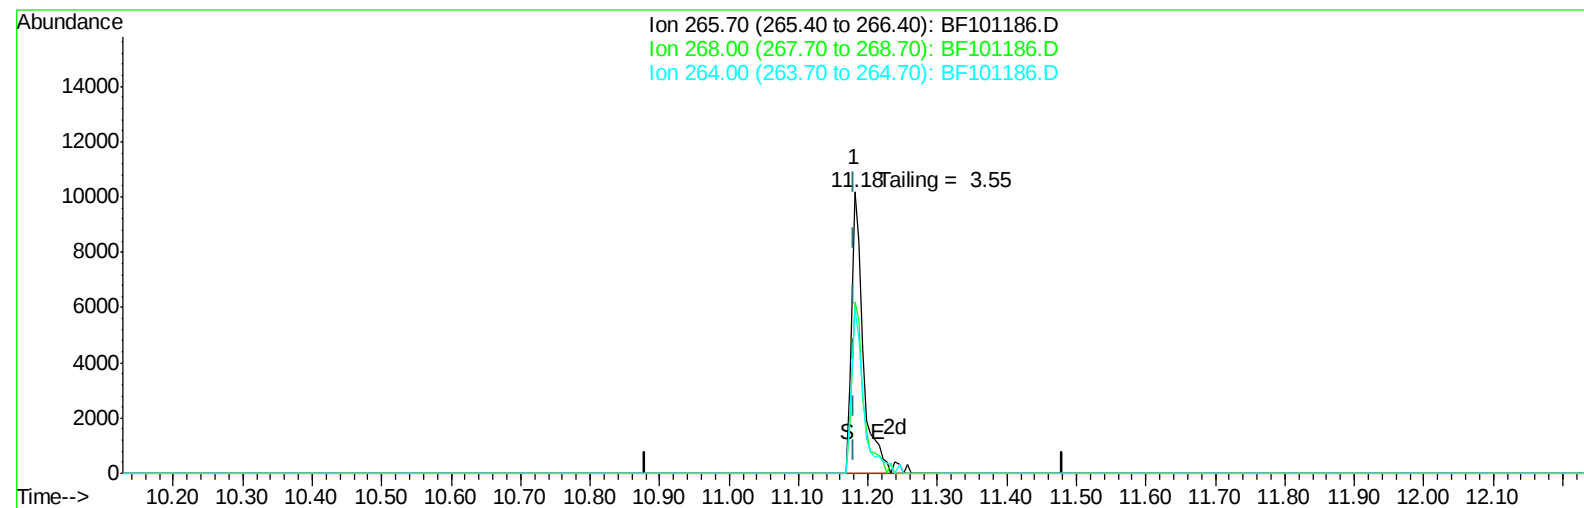

(69) Pentachlorophenol (C)



11.180min (+0.000) 0.00ng

response 11601

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.87
264.00	61.90	58.79
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF120617\
Data File : BF101186.D
Acq On : 7 Dec 2017 00:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:50:34 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:07:49 2017
Response via : Initial Calibration

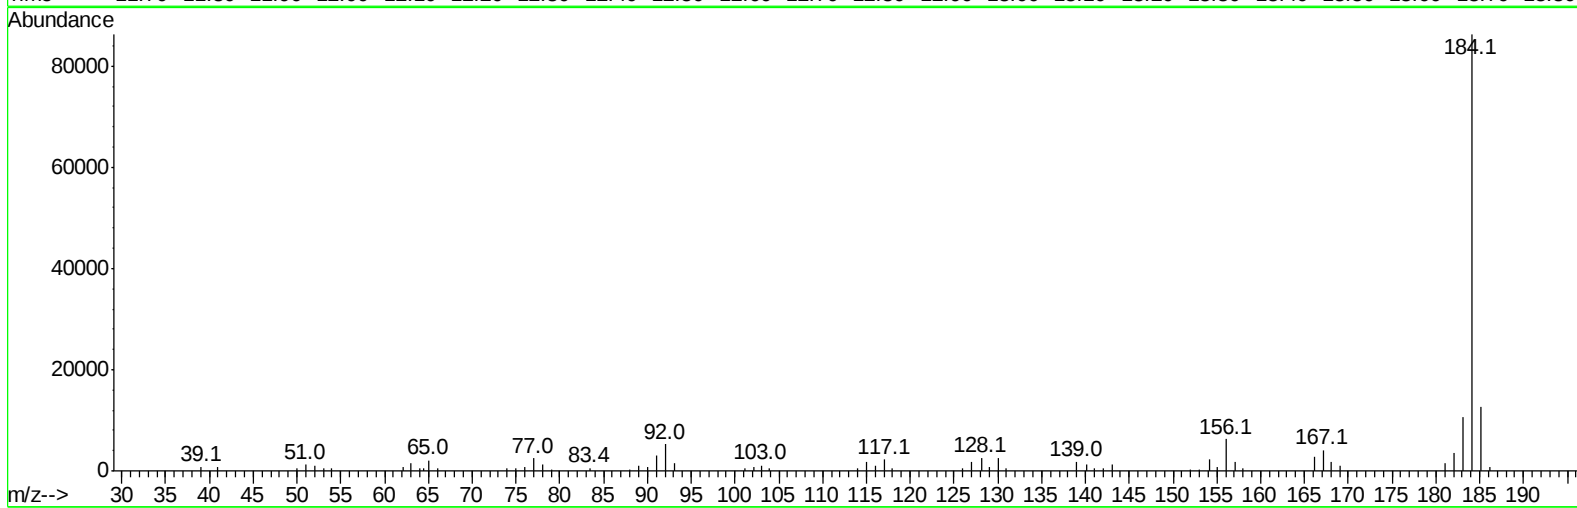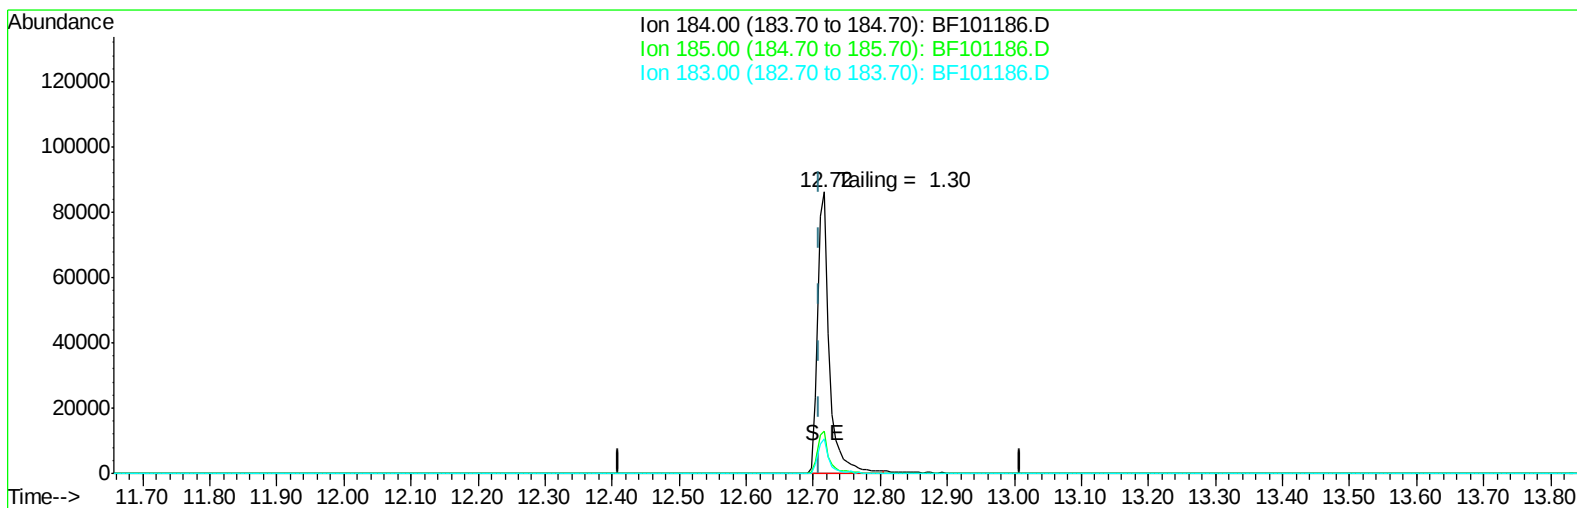

TIC: BF101186.D

(76) Benzidine

12.716min (+0.006) 0.00ng

response 102944

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.81
183.00	11.60	12.23
0.00	0.00	0.00