

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120617\
 Data File : BF101184.D
 Acq On : 6 Dec 2017 22:40
 Operator : SJ/JU
 Sample : I6722-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	505	508	520	rBV	41479	55607	5.35%	0.683%
2	5.469	571	575	591	rBV	980598	898518	86.48%	11.039%
3	6.481	742	747	764	rBV	908048	893982	86.04%	10.983%
4	6.616	766	770	774	rBV	1051221	952578	91.68%	11.703%
5	6.845	806	809	813	rBV	313014	257378	24.77%	3.162%
6	7.004	832	836	839	rBV	915383	737503	70.98%	9.061%
7	7.416	901	906	919	rBV	556989	549933	52.93%	6.756%
8	8.128	1024	1027	1034	rBV	390874	312554	30.08%	3.840%
9	9.204	1206	1210	1213	rBV	1305711	1039001	100.00%	12.765%
10	9.598	1273	1277	1284	rBV	138721	116124	11.18%	1.427%
11	9.886	1322	1326	1335	rVB	367809	311365	29.97%	3.825%
12	10.675	1457	1460	1470	rBV	520208	454910	43.78%	5.589%
13	10.775	1474	1477	1484	rBB	12830	14441	1.39%	0.177%
14	11.374	1575	1579	1586	rBV	314070	265930	25.59%	3.267%
15	12.957	1844	1848	1851	rBV	875665	738143	71.04%	9.069%
16	13.839	1995	1998	2002	rBV	22671	22580	2.17%	0.277%
17	14.021	2025	2029	2035	rBV	285583	268123	25.81%	3.294%
18	15.498	2274	2280	2287	rBV	193280	250719	24.13%	3.080%


Sum of corrected areas: 8139389

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120617\
Data File : BF101184.D
Acq On : 6 Dec 2017 22:40
Operator : SJ/JU
Sample : I6722-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

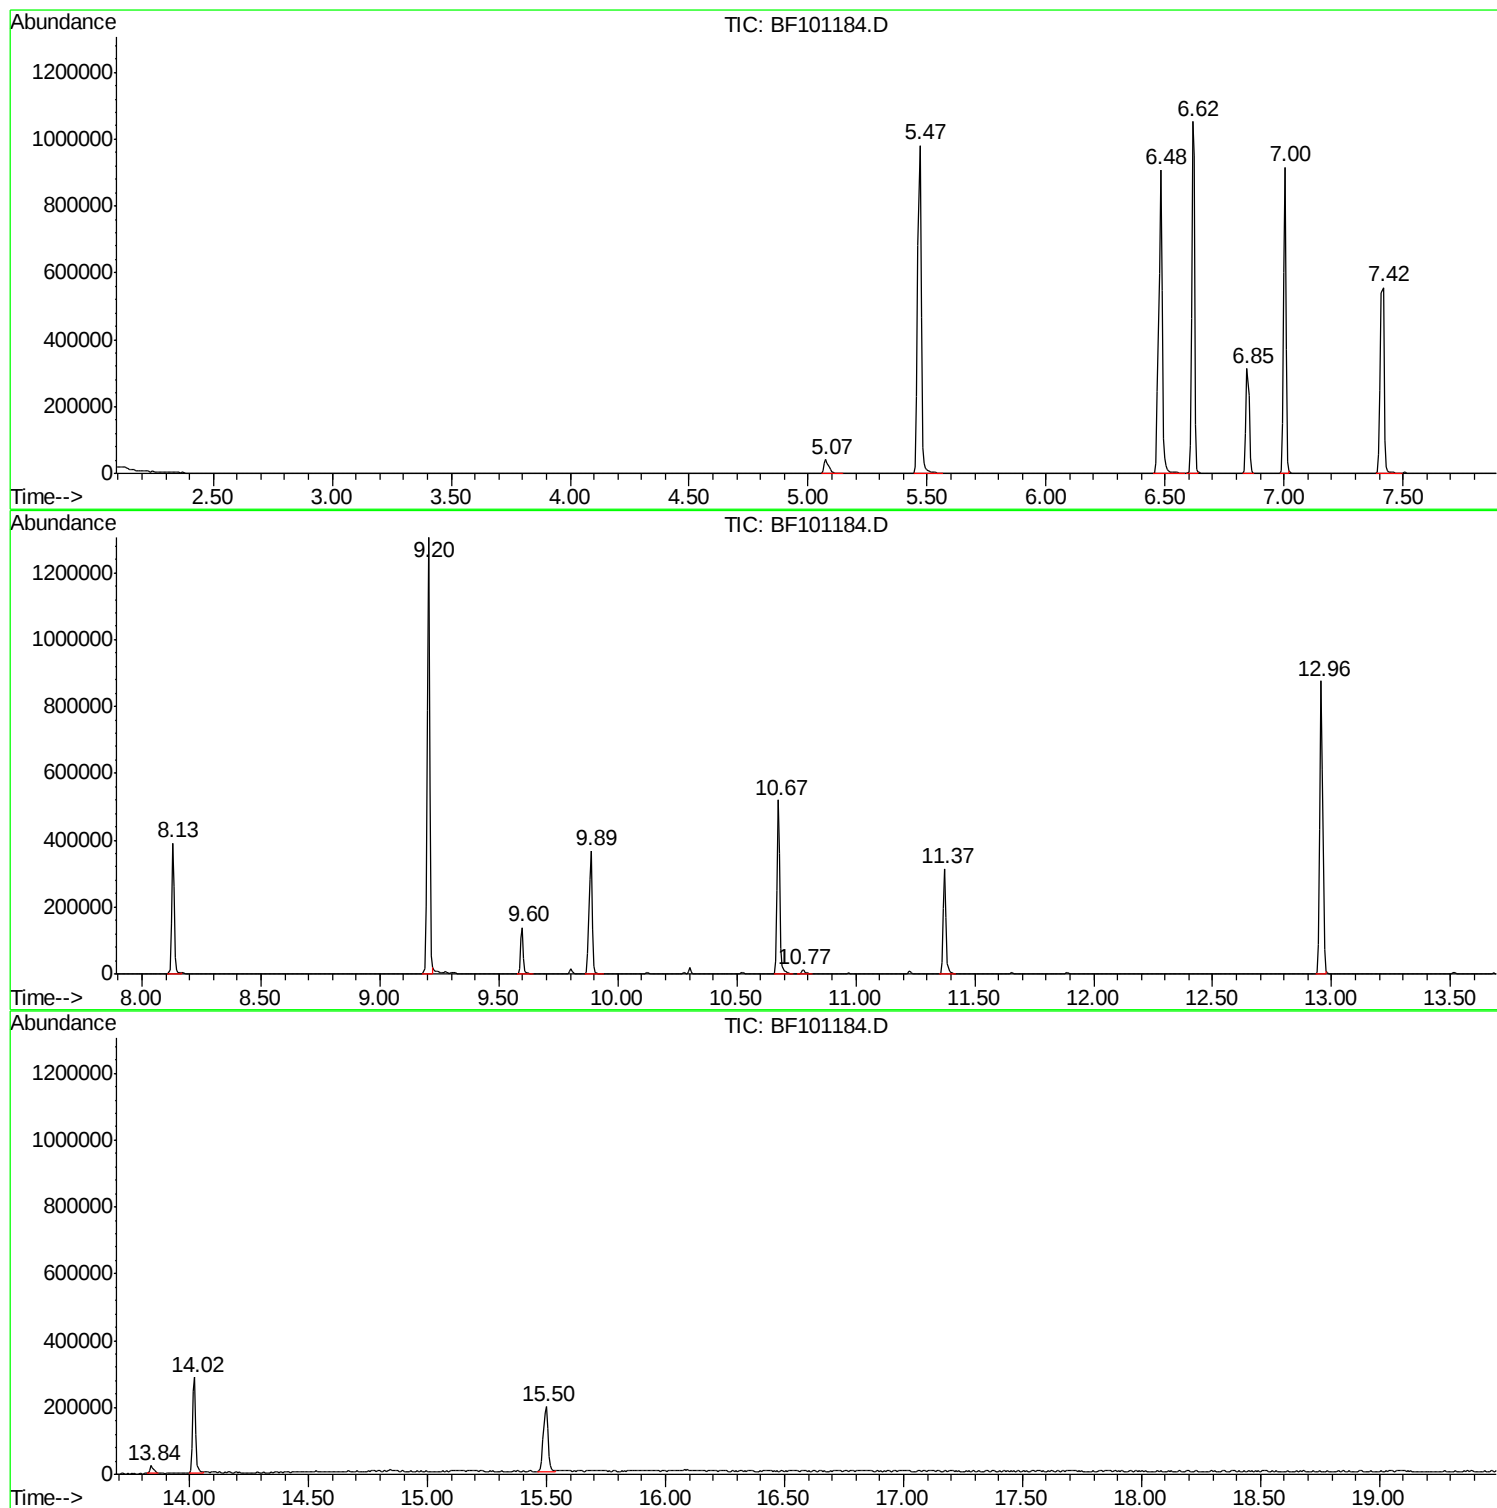

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120617\
Data File : BF101184.D
Acq On : 6 Dec 2017 22:40
Operator : SJ/JU
Sample : I6722-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.07	4.32 ng	55607	1,4-Dichlorobenzene-d4	6.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
3			2-Propanone, 1-(1-methylethoxy)-	116	C6H12O2	042781-12-4	9
4			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	9
5			4-Penten-2-one, 4-methyl-	98	C6H10O	003744-02-3	7

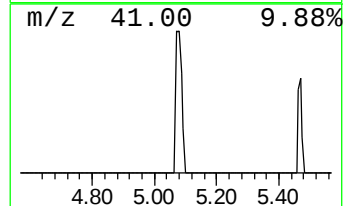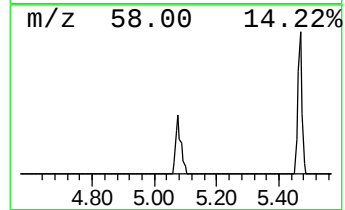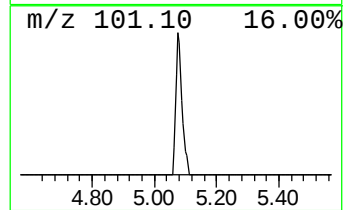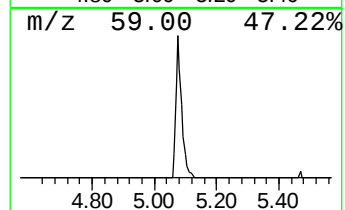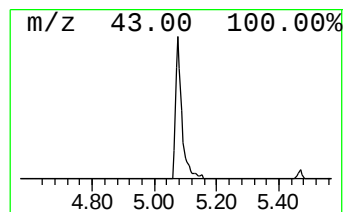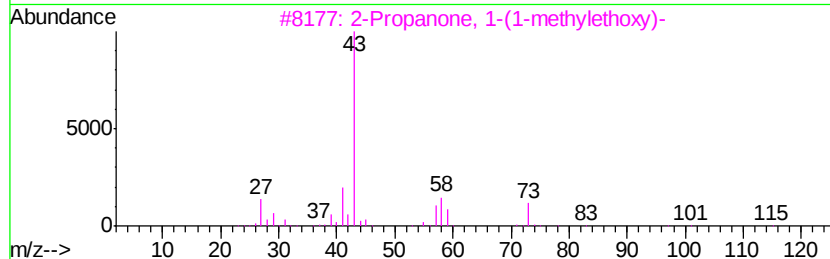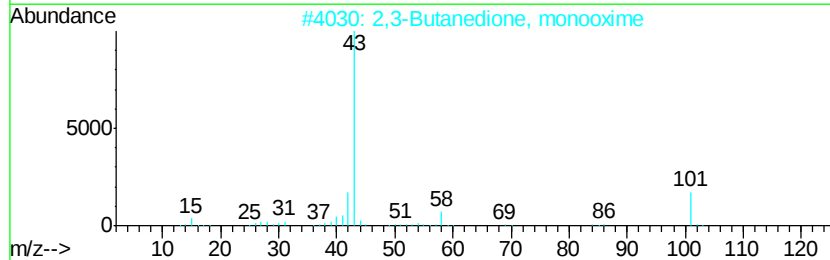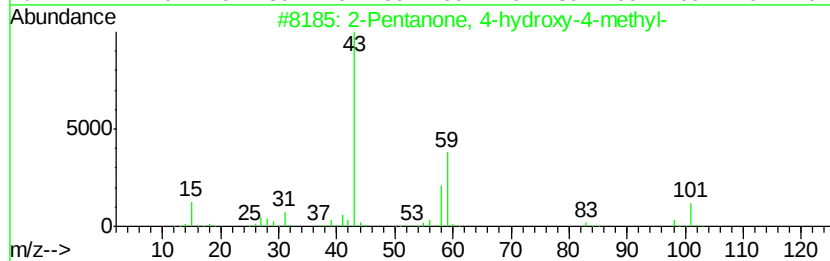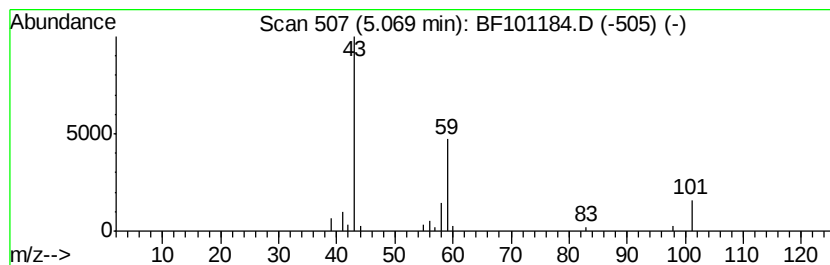

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120617\
Data File : BF101184.D
Acq On : 6 Dec 2017 22:40
Operator : SJ/JU
Sample : I6722-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	74.02 ng	952578	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	10
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

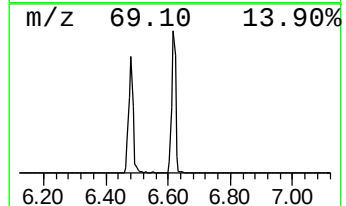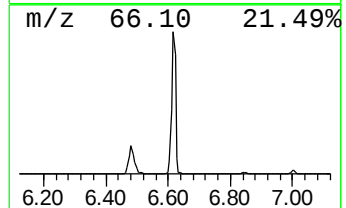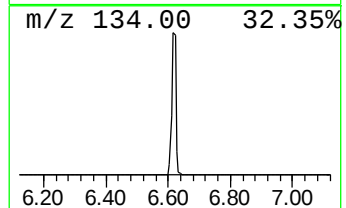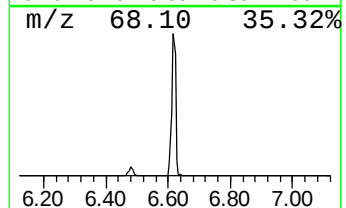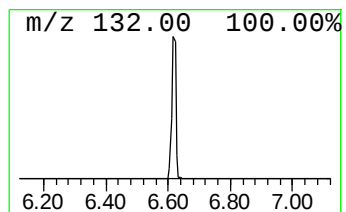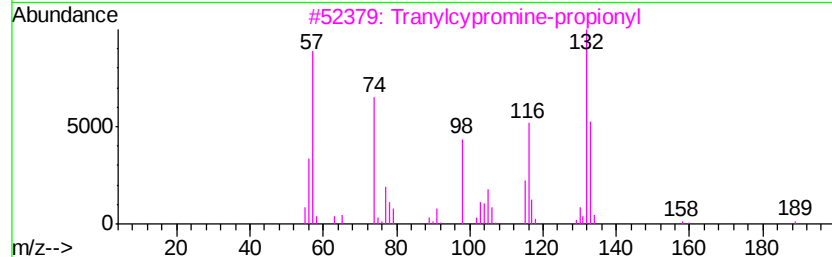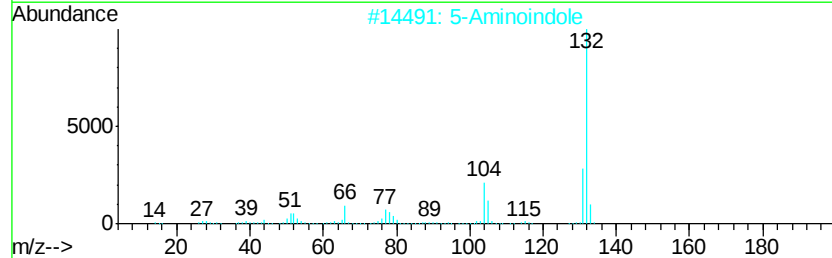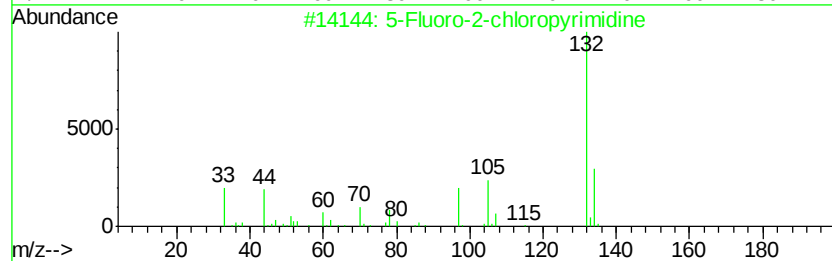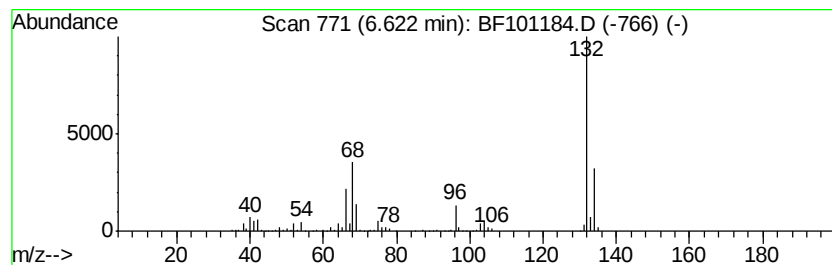

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120617\
Data File : BF101184.D
Acq On : 6 Dec 2017 22:40
Operator : SJ/JU
Sample : I6722-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.07	4.3	ng	55607	1	6.85	257378	20.0
unknown6.62	6.62	74.0	ng	952578	1	6.85	257378	20.0