
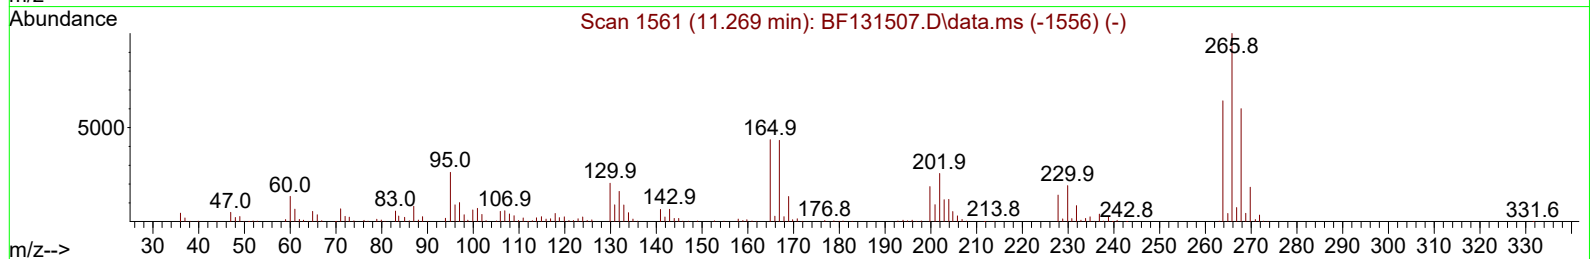
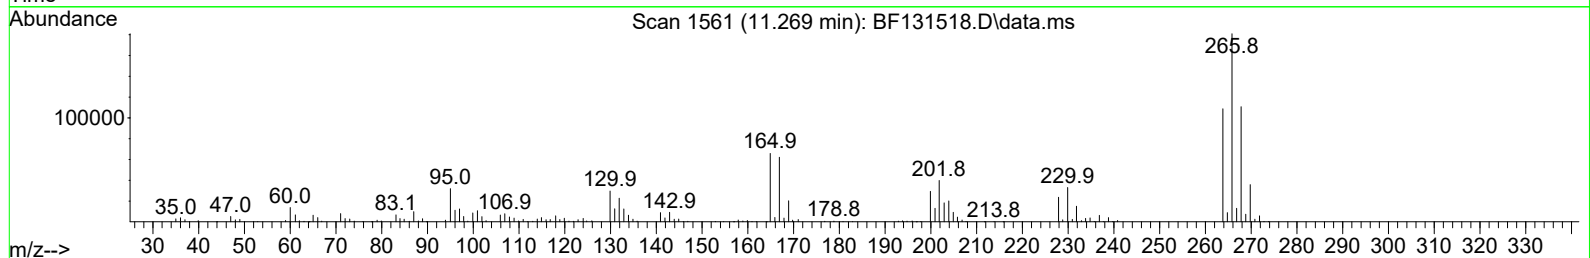


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120622\
 Data File : BF131518.D
 Acq On : 06 Dec 2022 09:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:14:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 01:30:30 2022
 Response via : Initial Calibration

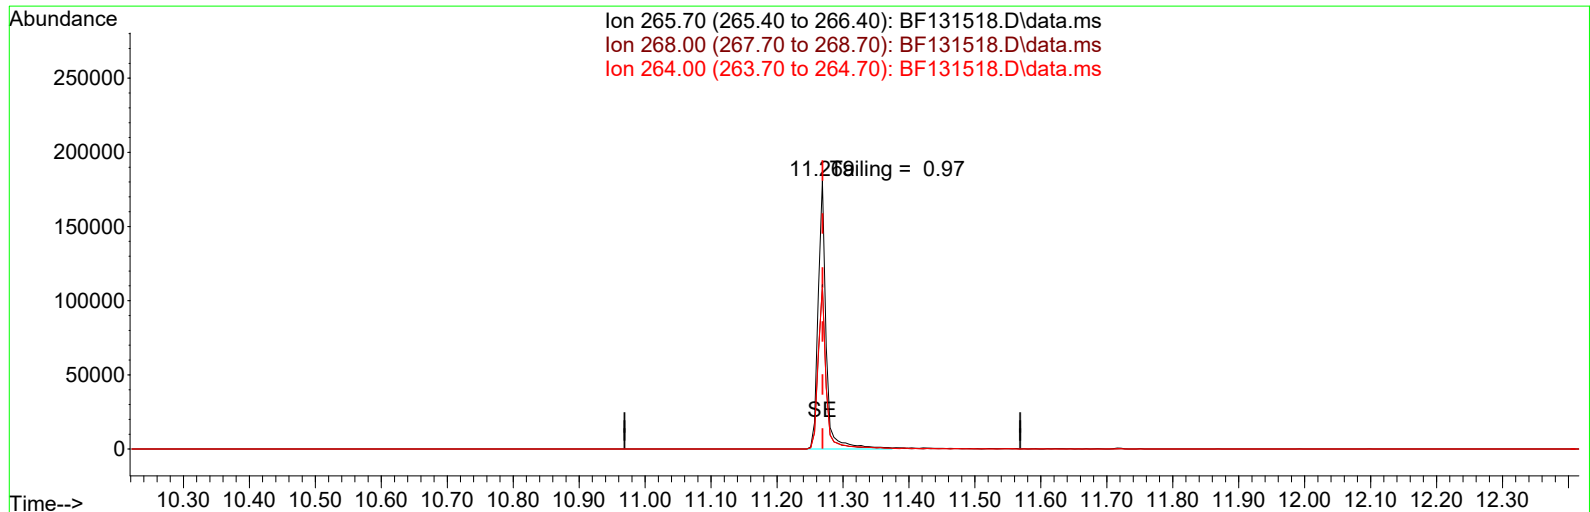

TIC: BF131518.D\data.ms

(70) Pentachlorophenol (C)




11.269min (-0.000) 33499.71 ng

response 153953

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.00	61.21
264.00	64.20	60.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120622\
Data File : BF131518.D
Acq On : 06 Dec 2022 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:14:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 01:30:30 2022
Response via : Initial Calibration

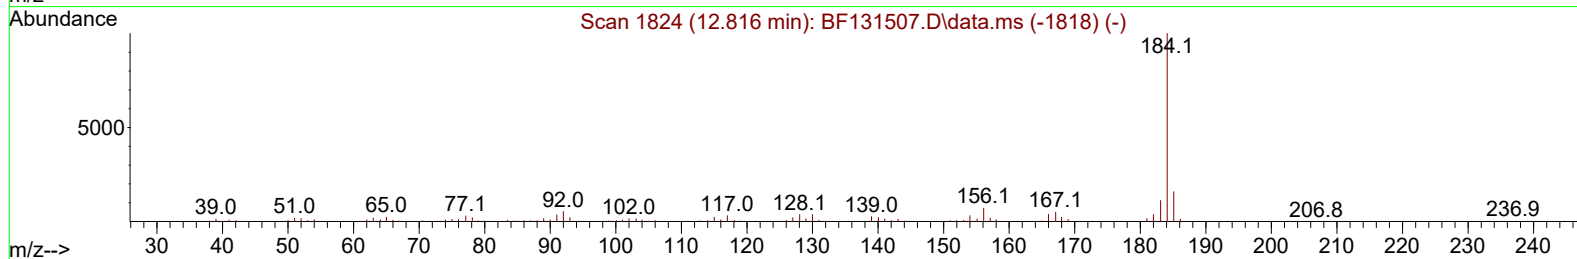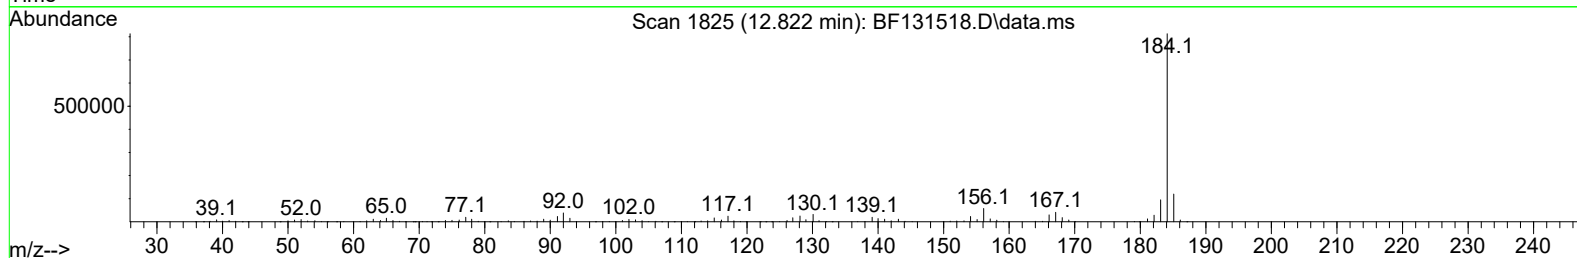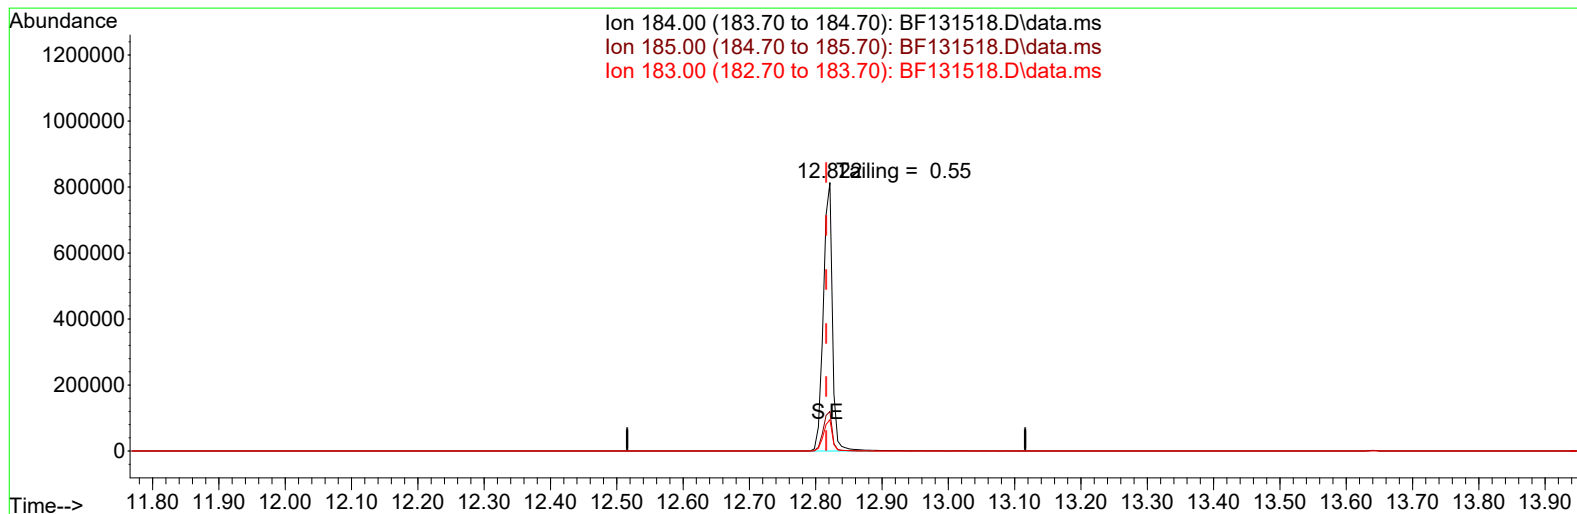

TIC: BF131518.D\data.ms

(77) Benzidine

12.822min (+ 0.006) 0.00 ng

response 778347

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.75
183.00	11.20	11.71
0.00	0.00	0.00