

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120622\
 Data File : BF131522.D
 Acq On : 06 Dec 2022 12:09
 Operator : CG\JU
 Sample : PB149413BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB149413BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF131522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.293	27	35	41	rVB	43801	61875	1.30%	0.268%
2	5.157	517	522	532	rBV	223019	311289	6.53%	1.348%
3	5.546	582	588	591	rBV	2624623	2646680	55.51%	11.462%
4	6.545	751	758	761	rBV	2317760	2634419	55.25%	11.409%
5	6.922	818	822	825	rBV	600915	521961	10.95%	2.260%
6	7.487	912	918	921	rBV	1545605	1741007	36.52%	7.540%
7	8.210	1035	1041	1044	rBV	742606	674039	14.14%	2.919%
8	9.292	1218	1225	1228	rBV	4248349	3969922	83.26%	17.192%
9	9.975	1335	1341	1344	rBV	993613	846752	17.76%	3.667%
10	10.769	1469	1476	1479	rBV	3079562	2632520	55.21%	11.400%
11	11.469	1589	1595	1598	rBV	1156526	928972	19.48%	4.023%
12	13.069	1861	1867	1870	rBV	5360312	4767880	100.00%	20.648%
13	14.121	2042	2046	2057	rBV	948691	785264	16.47%	3.401%
14	15.639	2299	2304	2315	rBV	422699	568703	11.93%	2.463%




Sum of corrected areas: 23091283

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120622\
Data File : BF131522.D
Acq On : 06 Dec 2022 12:09
Operator : CG\JU
Sample : PB149413BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149413BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

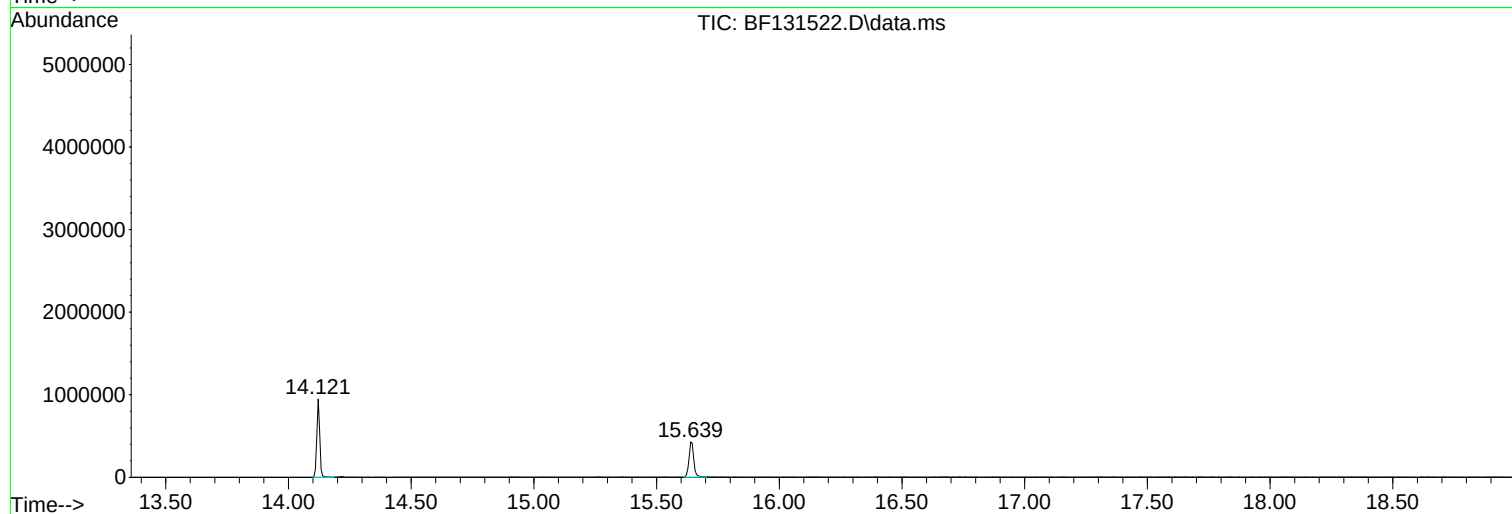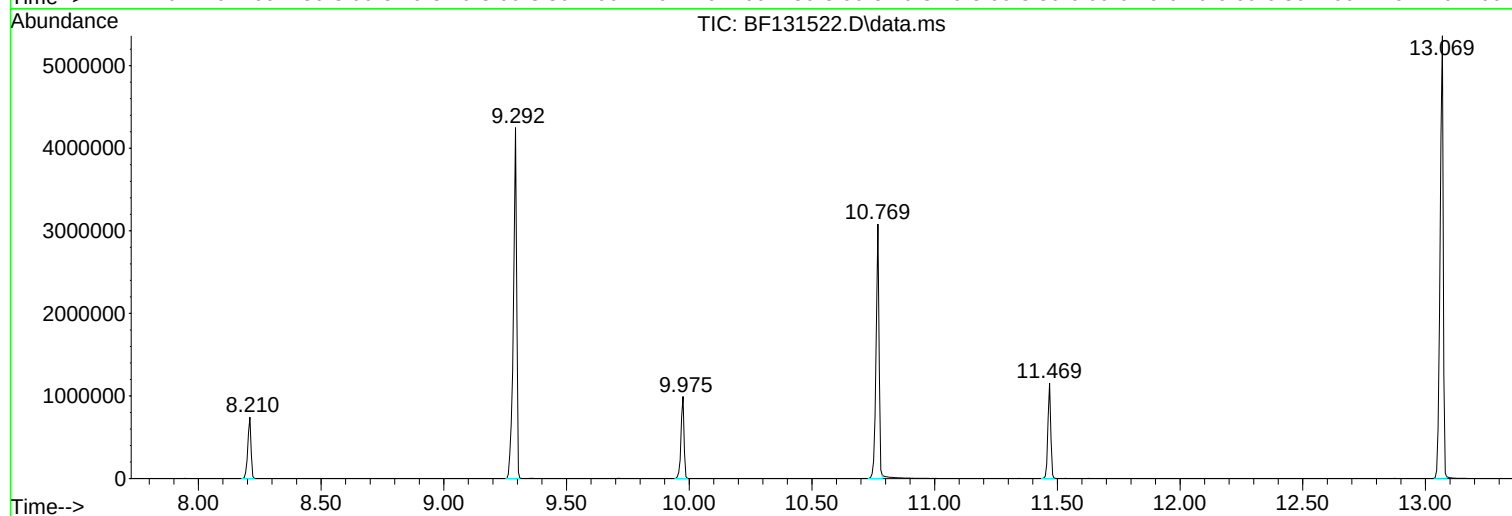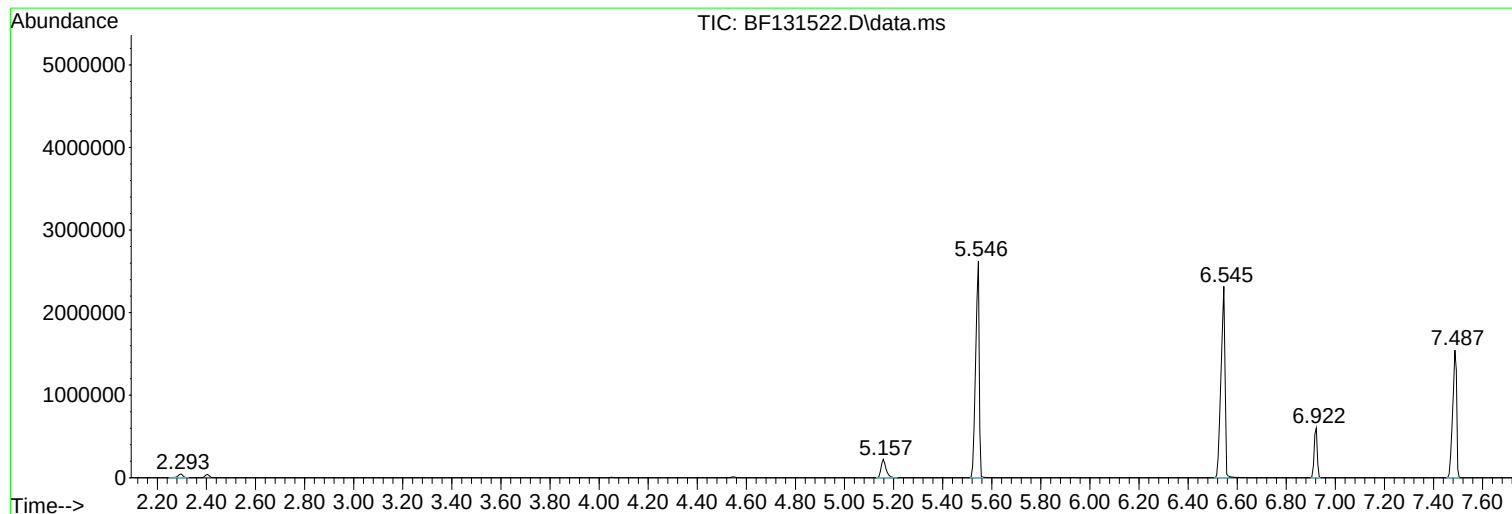

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120622\
Data File : BF131522.D
Acq On : 06 Dec 2022 12:09
Operator : CG\JU
Sample : PB149413BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149413BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.293	2.37 ng	61875	1,4-Dichlorobenzene-d4	6.922

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	23
4			N-Ethylformamide	73	C3H7NO	000627-45-2	9
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

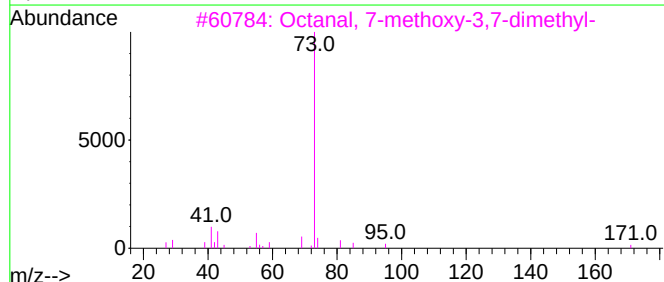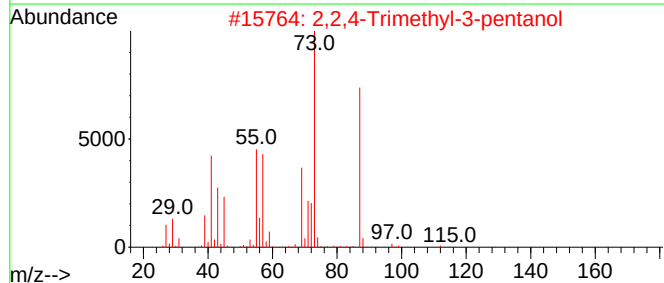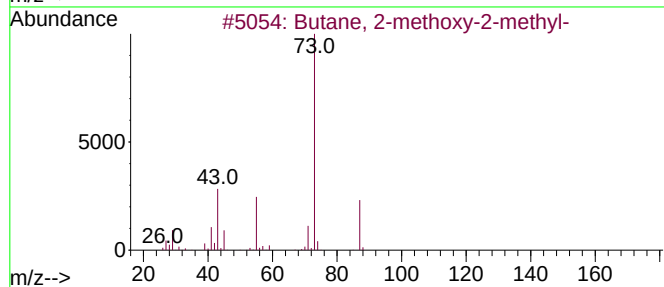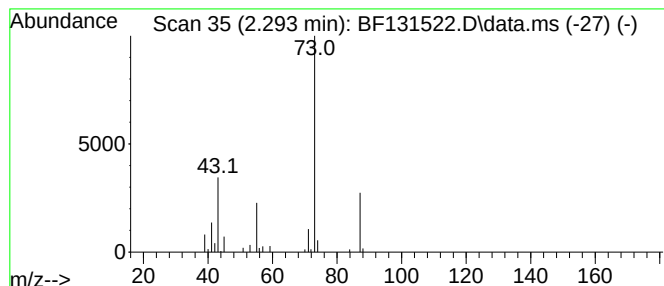

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120622\
Data File : BF131522.D
Acq On : 06 Dec 2022 12:09
Operator : CG\JU
Sample : PB149413BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149413BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.157	11.93 ng	311289	1,4-Dichlorobenzene-d4	6.922

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
4	5-Hexen-2-one	98	C6H10O	000109-49-9	9		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

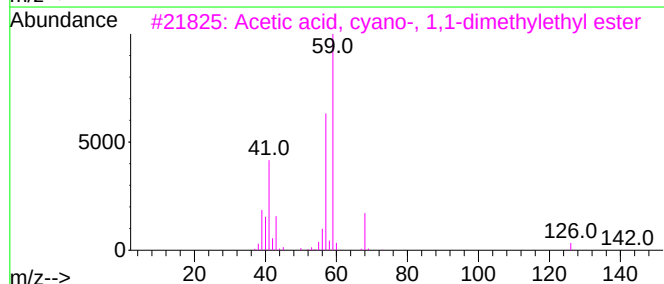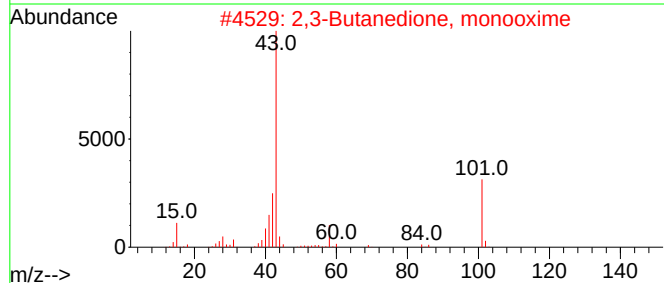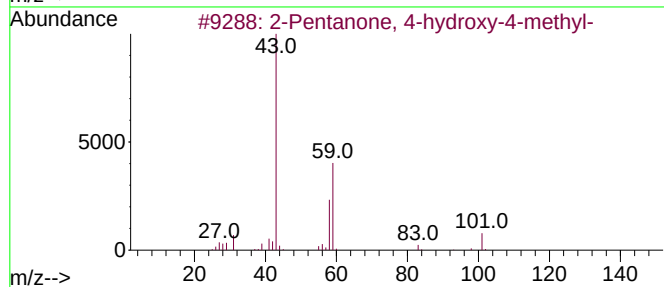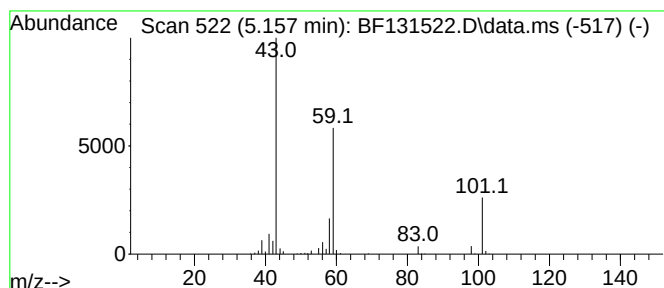

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120622\
Data File : BF131522.D
Acq On : 06 Dec 2022 12:09
Operator : CG\JU
Sample : PB149413BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149413BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.293	2.4	ng	61875	1	6.922	521961	20.0
2-Pentanone, 4-...	5.157	11.9	ng	311289	1	6.922	521961	20.0