
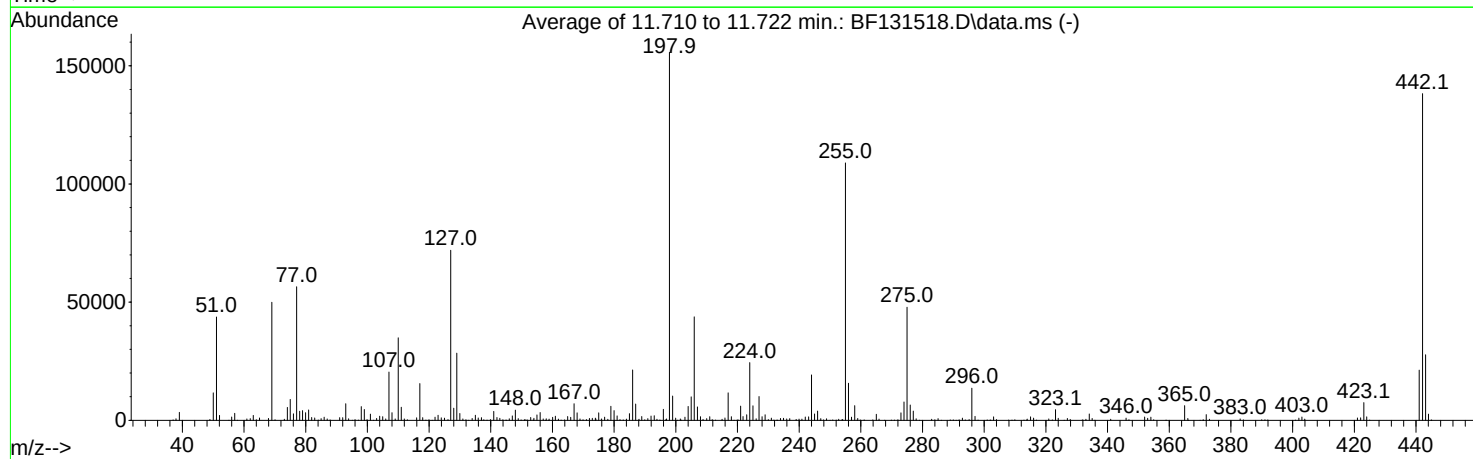


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120622\
 Data File : BF131518.D
 Acq On : 06 Dec 2022 09:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 06 01:30:30 2022

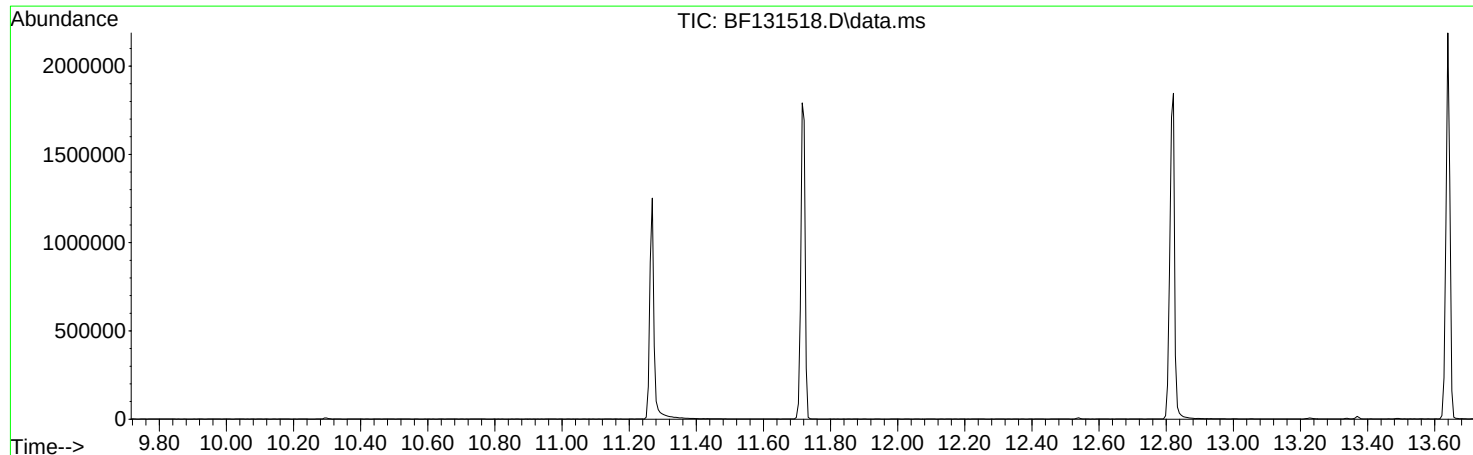




AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	43709	PASS
68	69	0.00	2	1.6	808	PASS
69	198	0.00	100	32.1	49933	PASS
70	69	0.00	2	0.5	237	PASS
127	198	10	80	46.2	71968	PASS
197	198	0.00	2	0.4	567	PASS
198	198	100	100	100.0	155669	PASS
199	198	5	9	6.6	10263	PASS
275	198	10	60	30.7	47861	PASS
365	198	1	100	4.0	6171	PASS
441	198	0.01	100	13.6	21201	PASS
442	442	50	100	100.0	138245	PASS
443	442	15	24	20.1	27725	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120622\
 Data File : BF131518.D
 Acq On : 06 Dec 2022 09:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 07 06:14:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 01:30:30 2022
 Response via : Initial Calibration

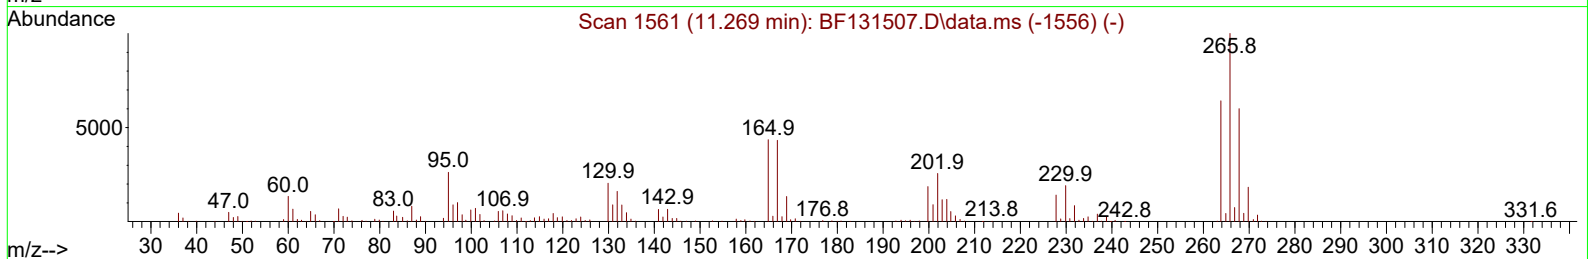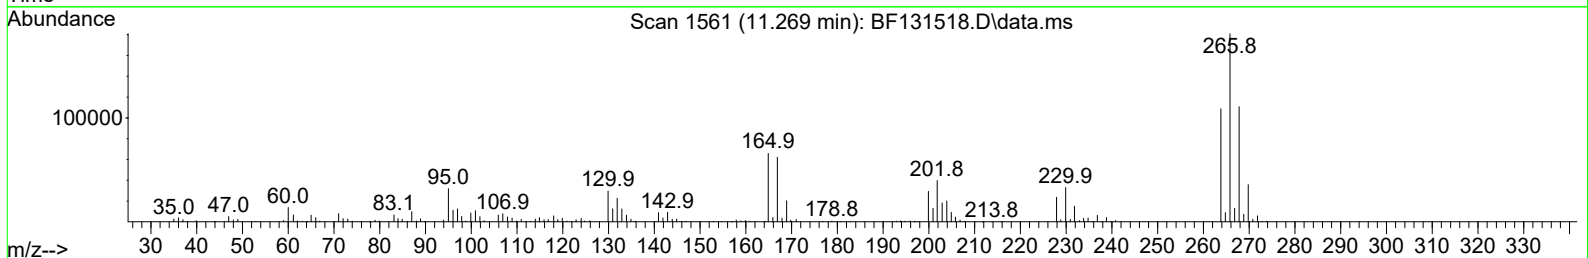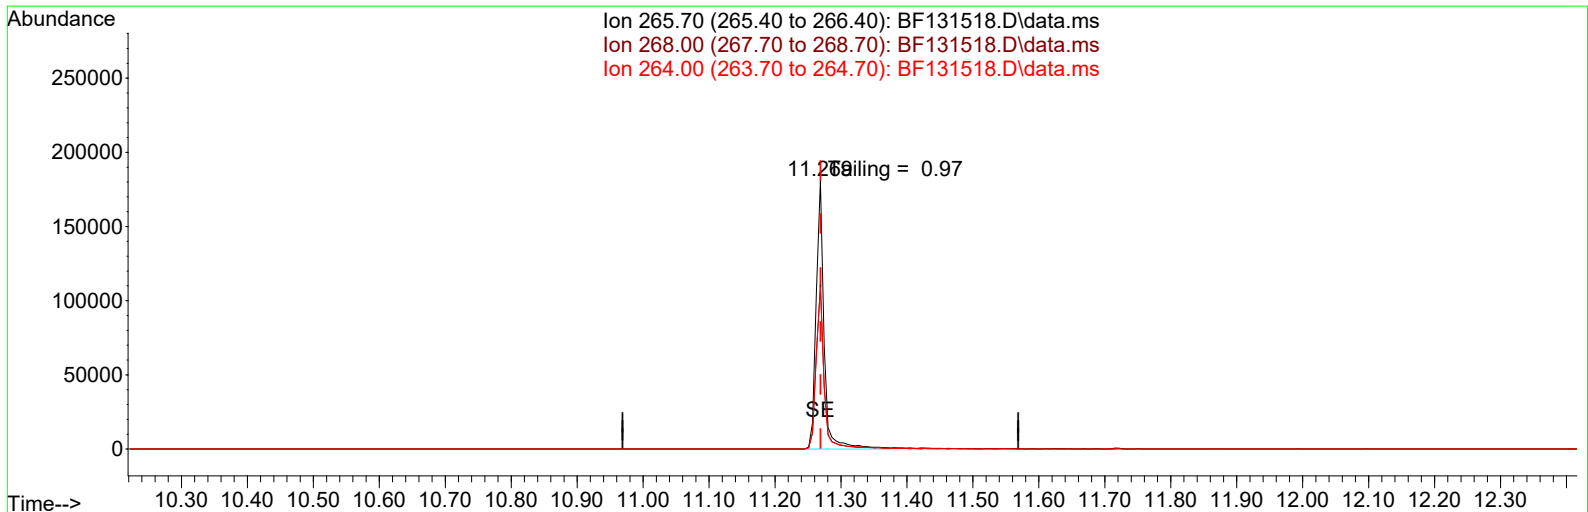

TIC: BF131518.D\data.ms

(70) Pentachlorophenol (C)

11.269min (-0.000) 33499.71 ng




response 153953

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.00	61.21
264.00	64.20	60.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120622\
Data File : BF131518.D
Acq On : 06 Dec 2022 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 07 06:14:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 01:30:30 2022
Response via : Initial Calibration

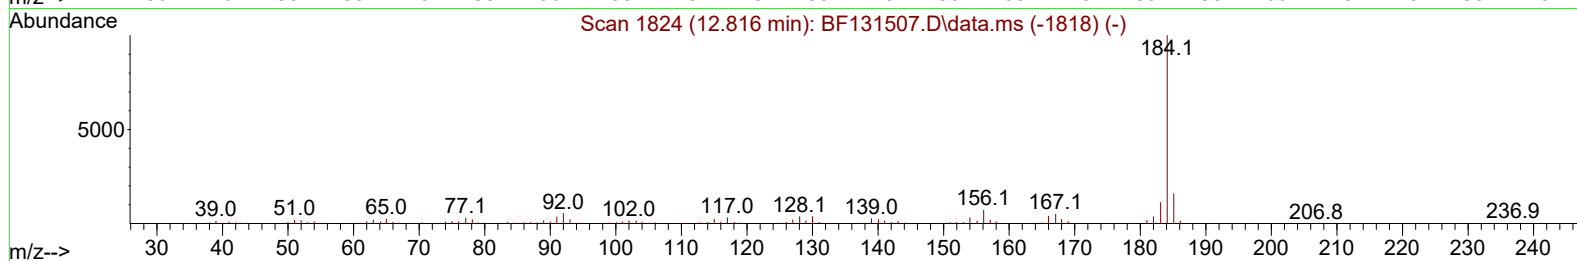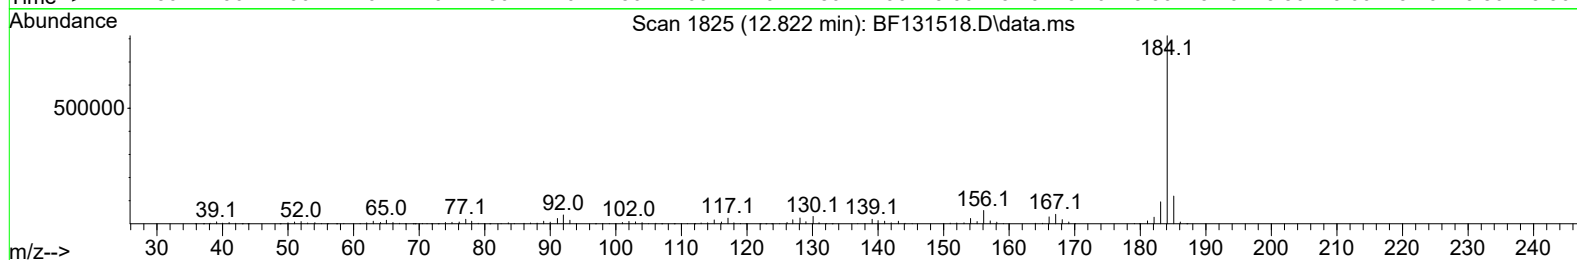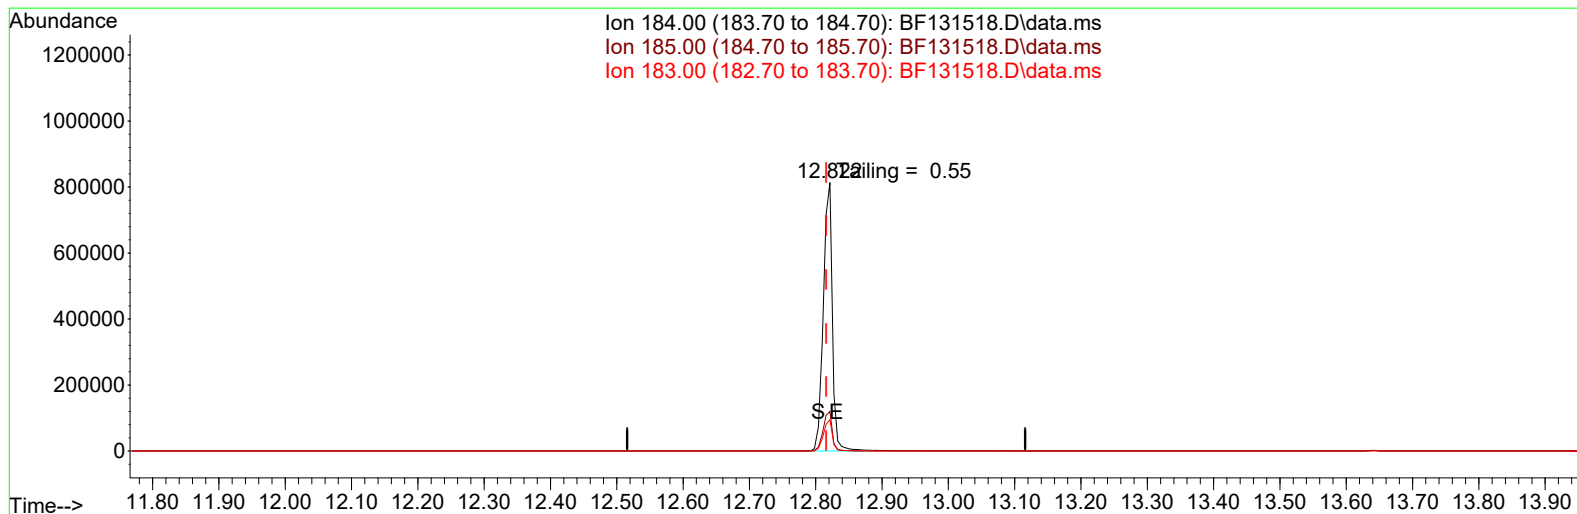

TIC: BF131518.D\data.ms

(77) Benzidine

12.822min (+ 0.006) 0.00 ng

response 778347

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.75
183.00	11.20	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/6/2022	BNA_F	<u>BF131518.D</u>
Compound Name	Response	Retention Time
DDT	364181	13.639
DDD	3875	13.369
DDE	160	12.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4035	368216	1.10

Instrument :
BNA_F
ClientSampleId :
DFTPP