
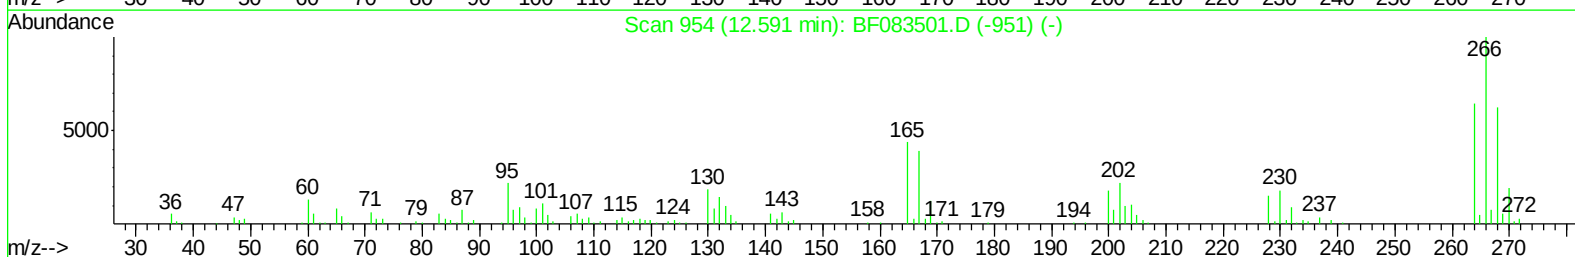
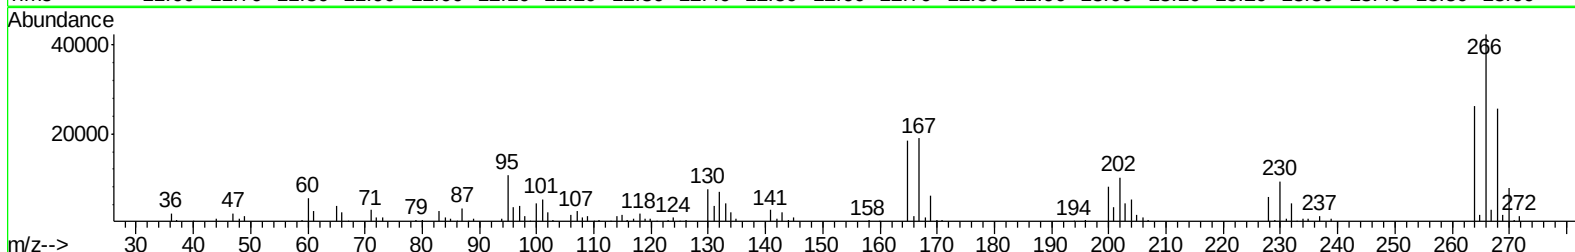


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120715\
Data File : BF083557.D
Acq On : 7 Dec 2015 13:49
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 08:32:14 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 05 04:12:46 2015
Response via : Initial Calibration

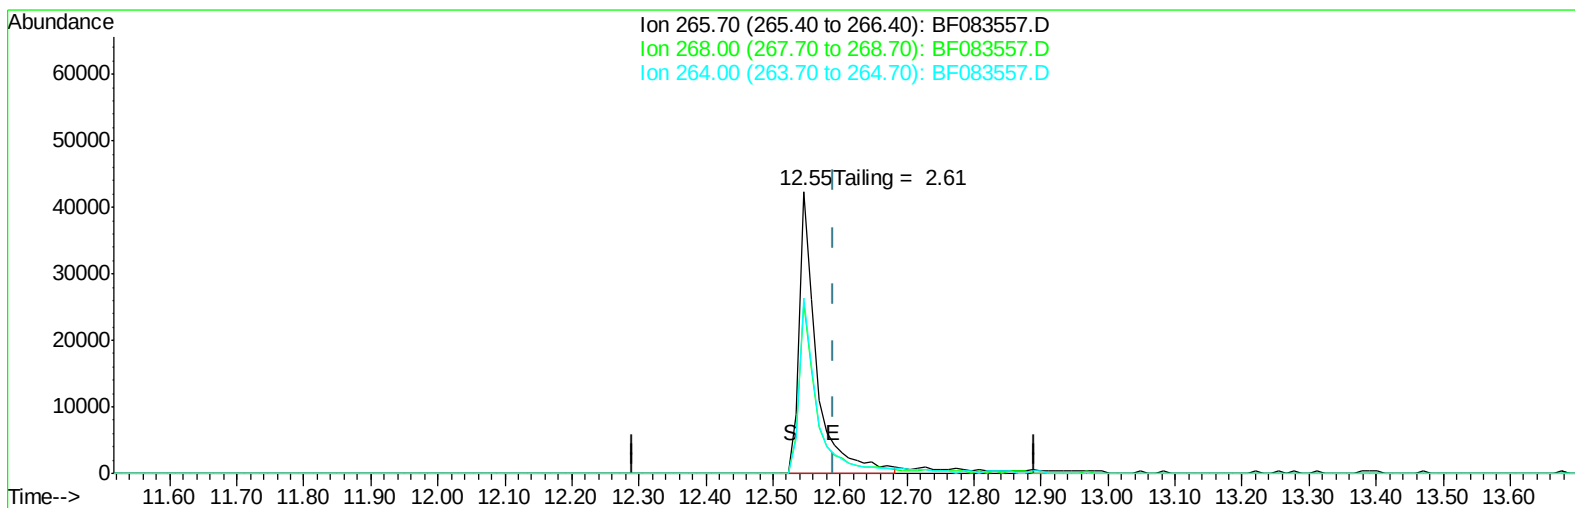

TIC: BF083557.D

(69) Pentachlorophenol (C)




12.545min (-0.045) 0.00ng

response 77986

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	60.28
264.00	64.30	62.17
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF120715\
Data File : BF083557.D
Acq On : 7 Dec 2015 13:49
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 08:32:14 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 05 04:12:46 2015
Response via : Initial Calibration

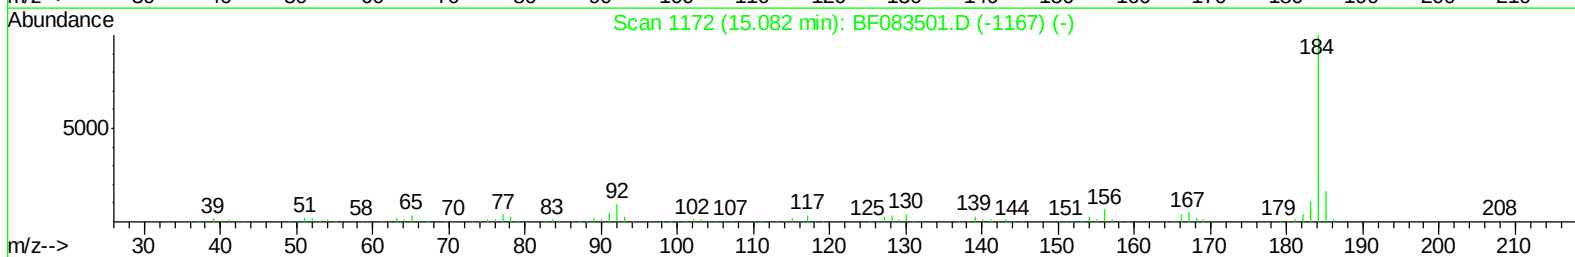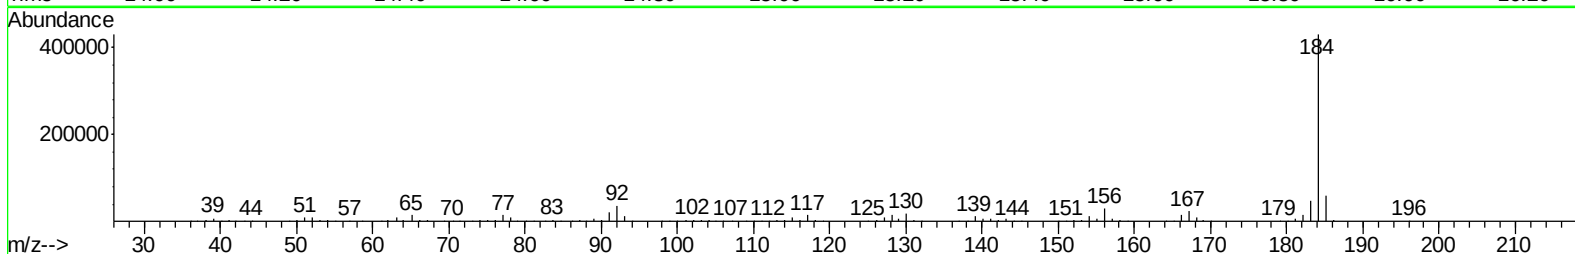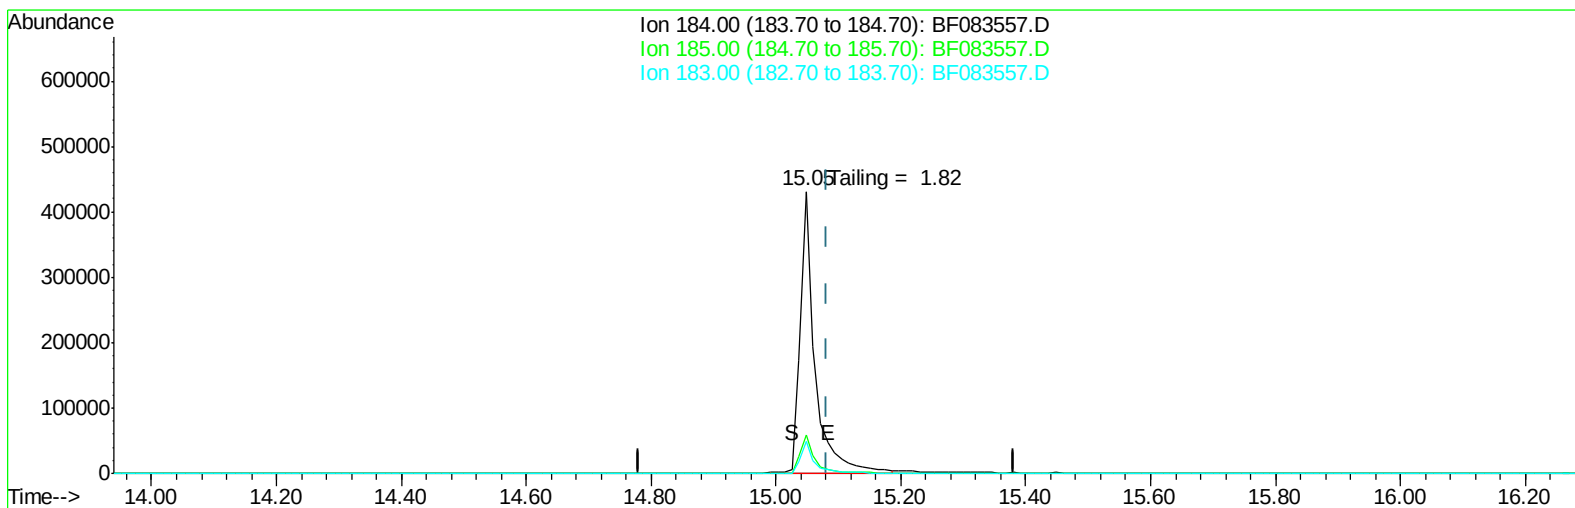

TIC: BF083557.D

(76) Benzidine

15.048min (-0.034) 0.00ng

response 735598

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.69
183.00	11.20	11.18
0.00	0.00	0.00