

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120715\
 Data File : BF083564.D
 Acq On : 7 Dec 2015 18:59
 Operator : UM/IZ
 Sample : G4579-01 20X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP1(6-12)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.561	162	164	174	rBV	23123	63173	5.07%	0.840%
2	4.030	202	205	219	rBV	47928	167318	13.42%	2.226%
3	5.310	315	317	326	rBV5	63731	178951	14.35%	2.381%
4	5.436	326	328	339	rVB	136449	241016	19.33%	3.206%
5	5.721	351	353	363	rBV	625059	837415	67.17%	11.141%
6	5.950	370	373	380	rBV	88670	159325	12.78%	2.120%
7	6.579	425	428	440	rBV	36864	123862	9.94%	1.648%
8	7.619	517	519	535	rBV	728909	1116023	89.52%	14.847%
9	9.367	670	672	683	rVB	145093	210135	16.86%	2.796%
10	10.065	730	733	743	rVB	21452	43827	3.52%	0.583%
11	10.408	760	763	778	rBV	869970	1246664	100.00%	16.585%
12	11.722	875	878	883	rBV	41594	87436	7.01%	1.163%
13	12.031	902	905	910	rBV2	7578	15730	1.26%	0.209%
14	12.808	970	973	984	rBV	810790	1158855	92.96%	15.417%
15	15.437	1201	1203	1209	rBV	102431	145742	11.69%	1.939%
16	16.317	1279	1280	1284	rBV2	7772	13406	1.08%	0.178%
17	16.945	1332	1335	1339	rBV2	11295	23078	1.85%	0.307%
18	17.014	1339	1341	1353	rBV	583209	852346	68.37%	11.339%
19	18.431	1463	1465	1468	rBV3	10864	21714	1.74%	0.289%
20	18.648	1482	1484	1491	rBV	486196	776654	62.30%	10.332%
21	19.506	1557	1559	1562	rVB3	12838	14381	1.15%	0.191%
22	19.963	1597	1599	1602	rBV3	11840	19671	1.58%	0.262%


Sum of corrected areas: 7516722

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120715\
Data File : BF083564.D
Acq On : 7 Dec 2015 18:59
Operator : UM/IZ
Sample : G4579-01 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP1(6-12)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

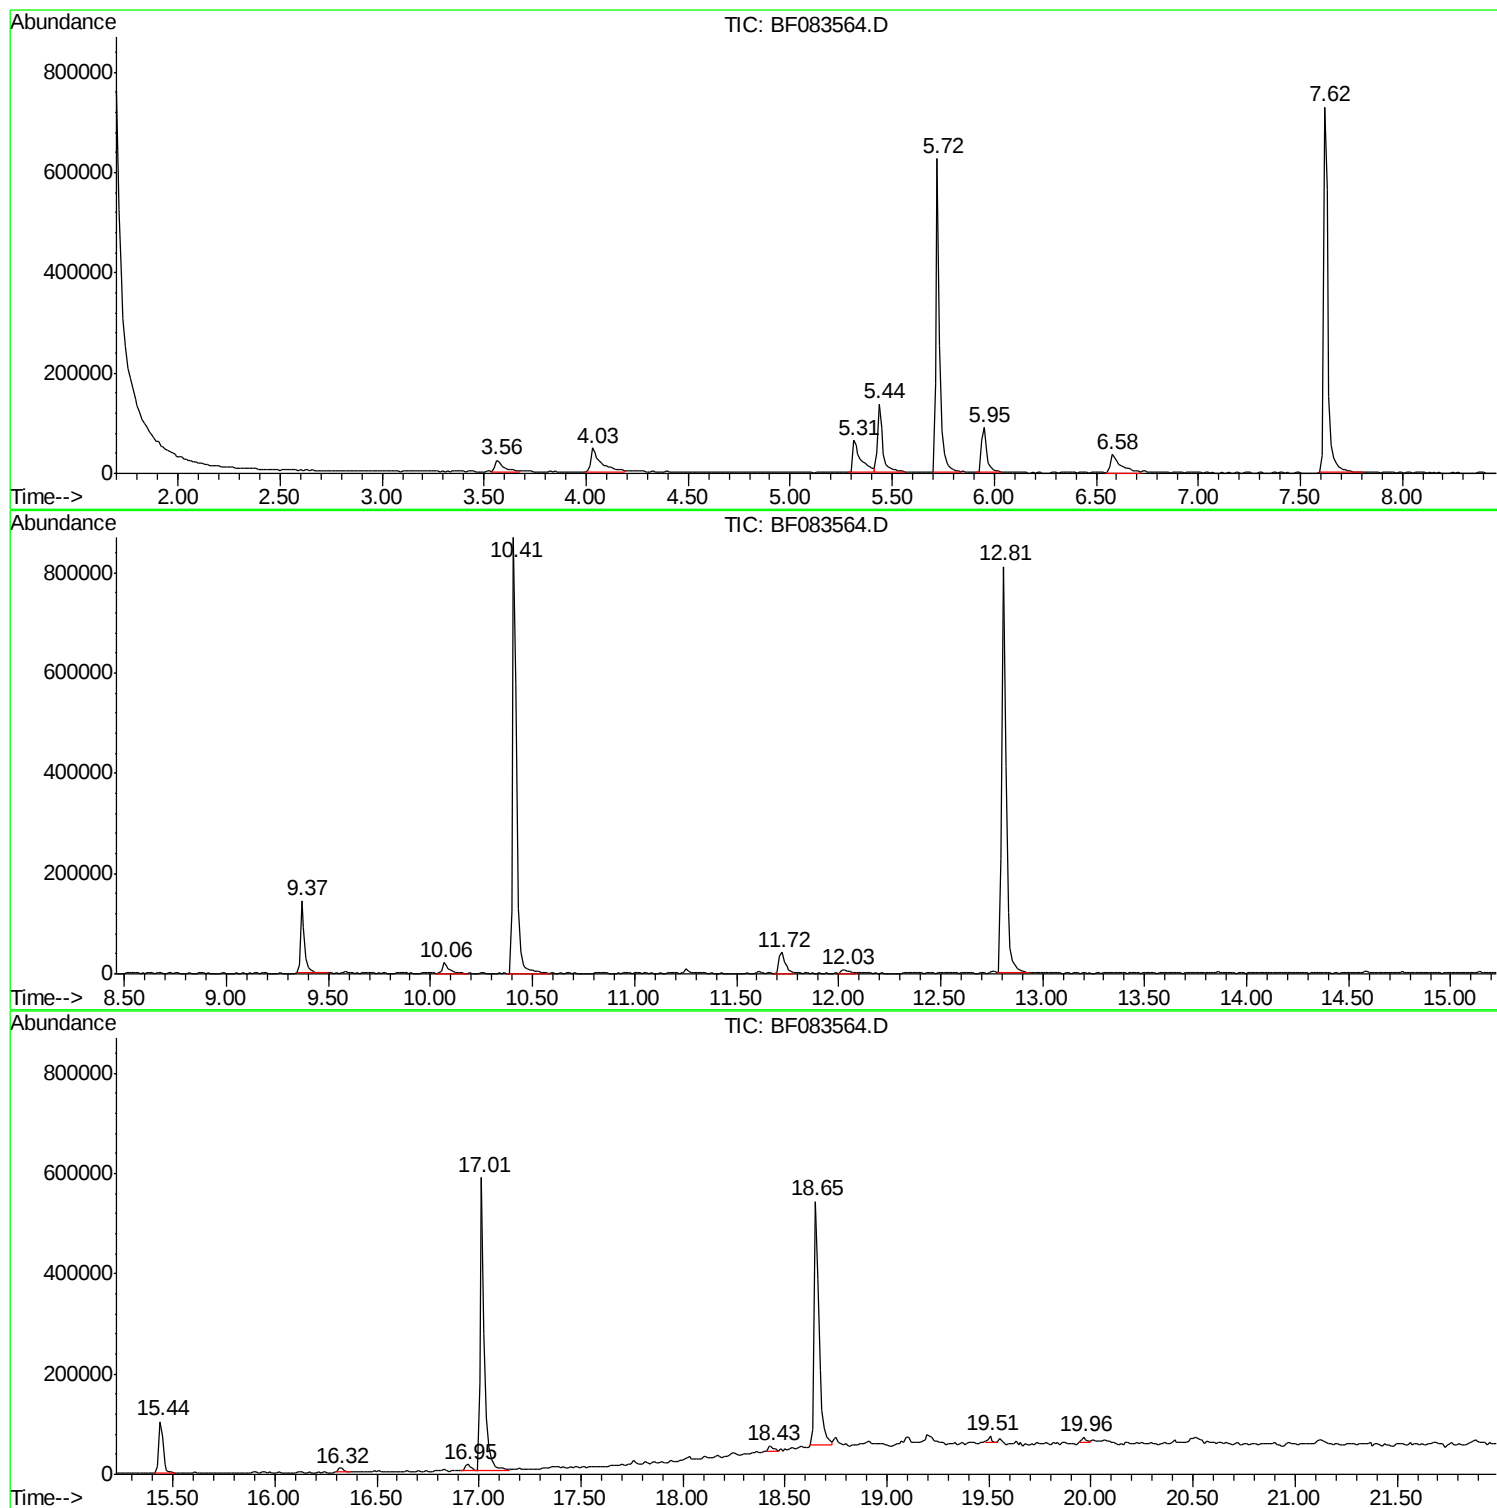

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120715\
Data File : BF083564.D
Acq On : 7 Dec 2015 18:59
Operator : UM/IZ
Sample : G4579-01 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP1(6-12)










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.44 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.44	5.76 ng	241016	1,4-Dichlorobenzene-d4	5.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Aminoindole	132	C8H8N2	005192-03-0	22
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		1H-Tetrazaborole, 5-chloro-4,5-d...	132	C2H6BClN4	021960-49-6	16
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	12
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

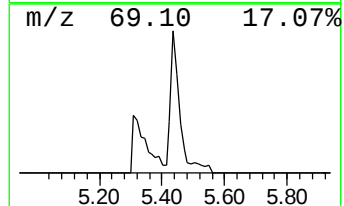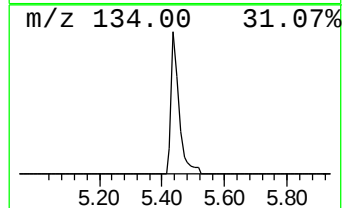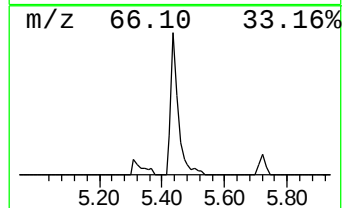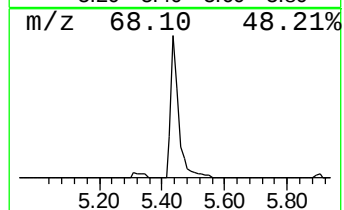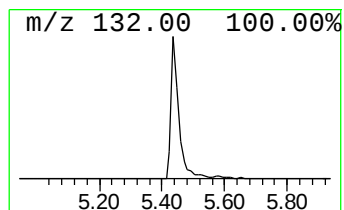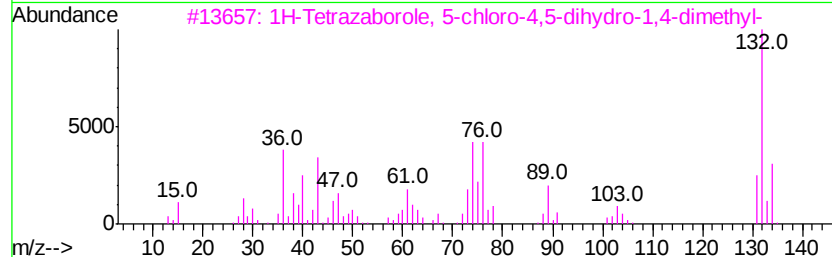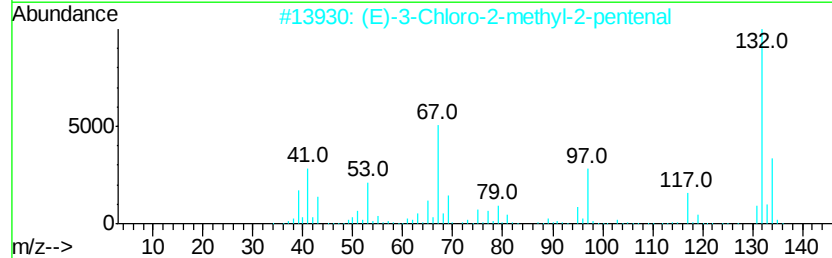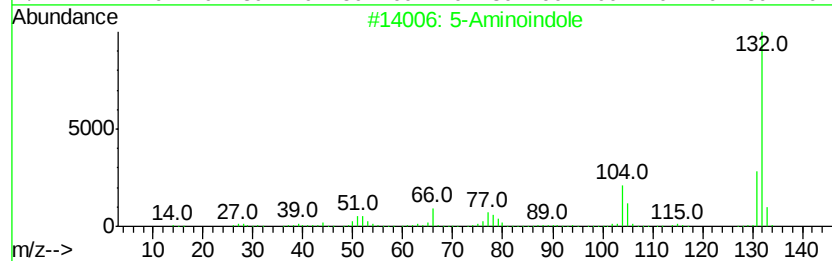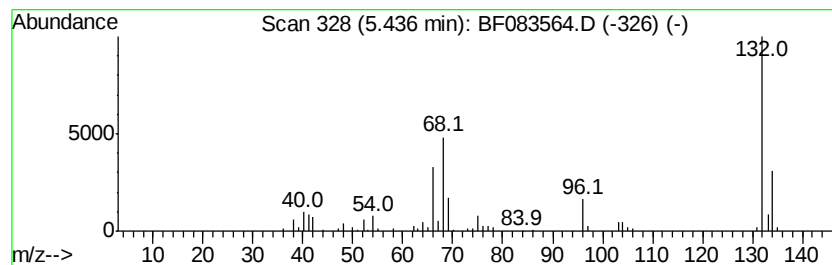

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120715\
Data File : BF083564.D
Acq On : 7 Dec 2015 18:59
Operator : UM/IZ
Sample : G4579-01 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP1(6-12)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.44	5.44	5.8	ng	241016	1	5.72	837415	20.0