


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120715\
 Data File : BF083557.D
 Acq On : 7 Dec 2015 13:49
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 05 04:12:46 2015

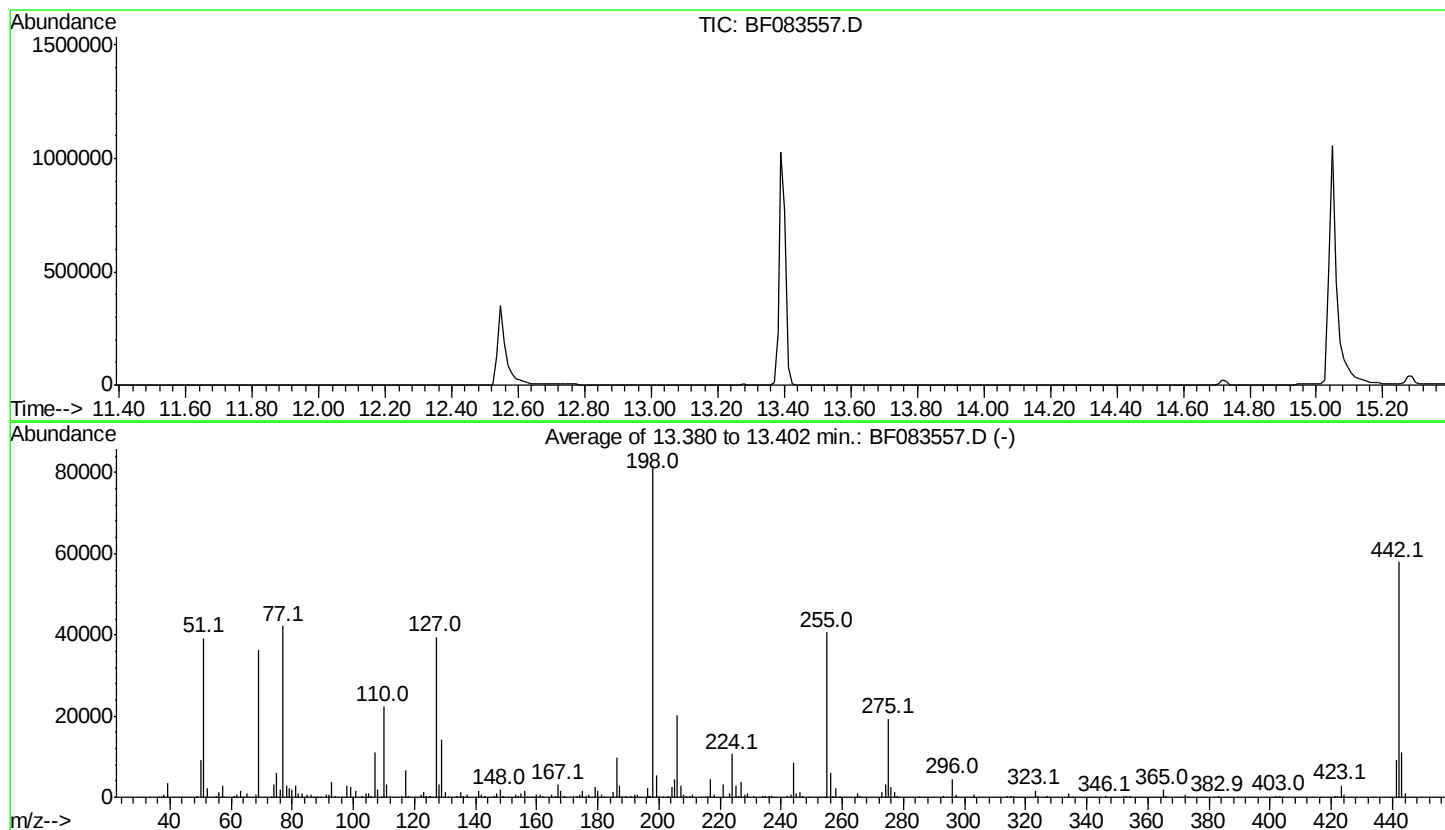

AutoFind: Scans 1023, 1024, 1025; Background Corrected with Scan 1019

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.0	39200	PASS
68	69	0.00	2	1.6	588	PASS
69	198	0.00	100	44.6	36437	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.4	39552	PASS
197	198	0.00	2	0.3	218	PASS
198	198	100	100	100.0	81714	PASS
199	198	5	9	6.5	5343	PASS
275	198	10	60	23.6	19286	PASS
365	198	1	100	2.2	1784	PASS
441	442	0.01	24	15.6	9060	PASS
442	198	50	100	71.0	57985	PASS
443	442	15	24	19.2	11150	PASS