


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120715\
 Data File : BF083578.D
 Acq On : 8 Dec 2015 2:42
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 05 04:12:46 2015

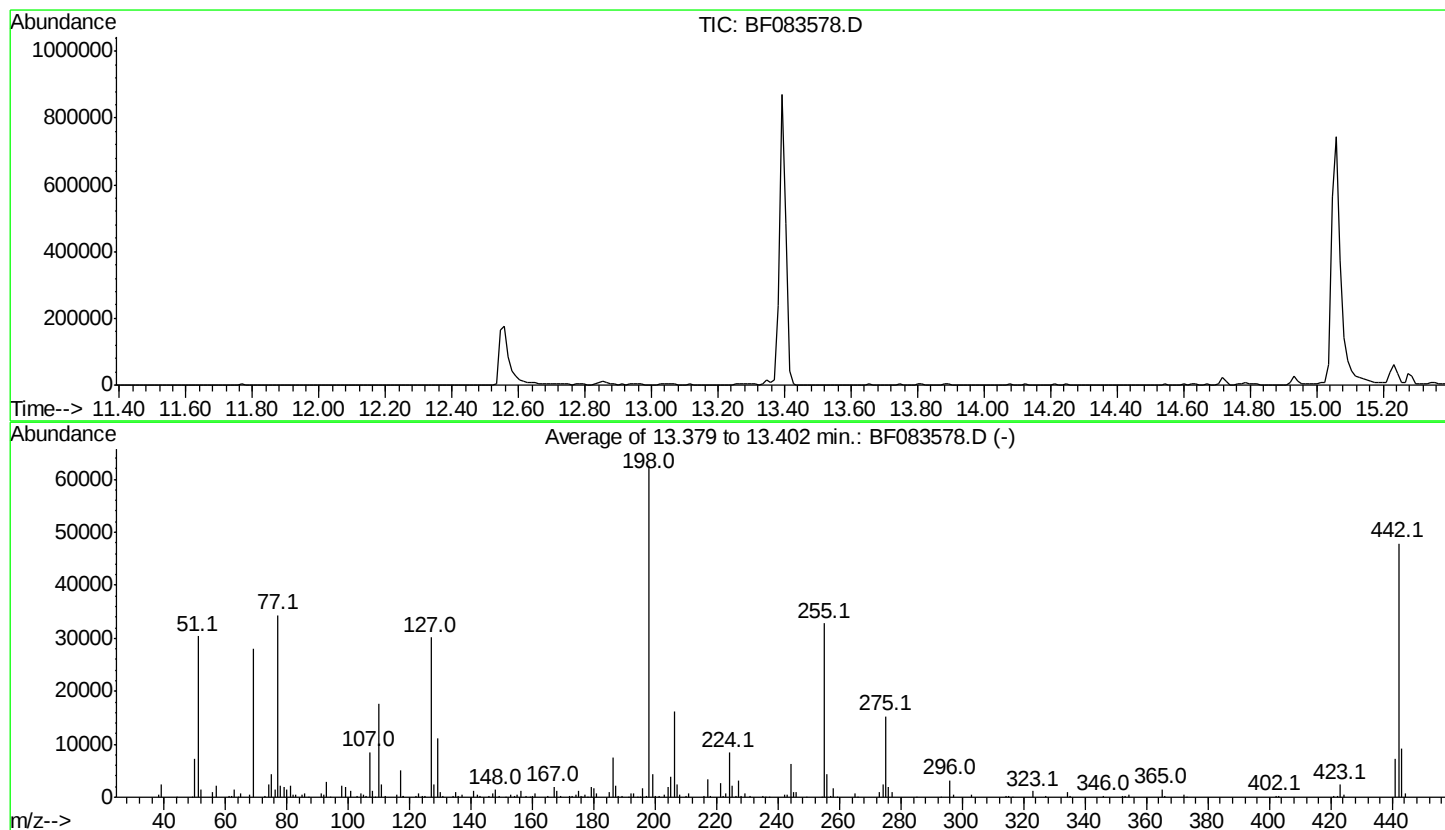

AutoFind: Scans 1023, 1024, 1025; Background Corrected with Scan 1019

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.6	30383	PASS
68	69	0.00	2	1.4	393	PASS
69	198	0.00	100	44.8	28022	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.2	30133	PASS
197	198	0.00	2	0.4	233	PASS
198	198	100	100	100.0	62573	PASS
199	198	5	9	7.0	4408	PASS
275	198	10	60	24.5	15311	PASS
365	198	1	100	2.5	1568	PASS
441	442	0.01	24	15.2	7285	PASS
442	198	50	100	76.5	47899	PASS
443	442	15	24	19.3	9240	PASS