
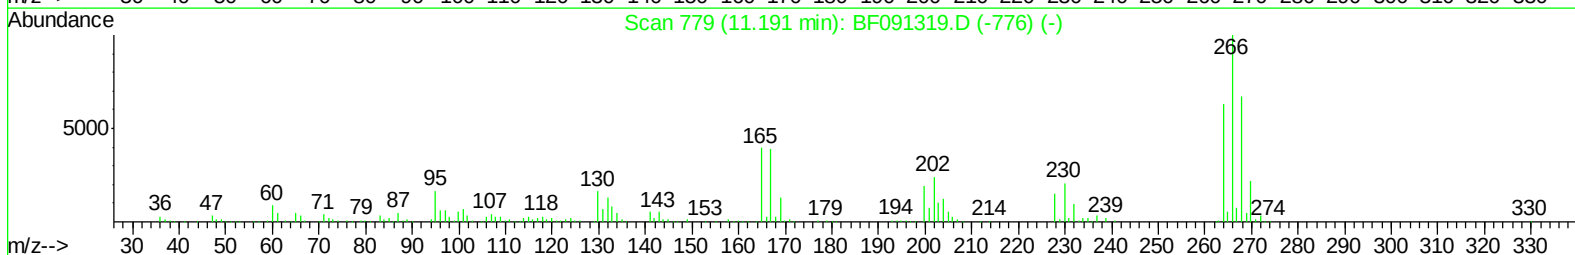
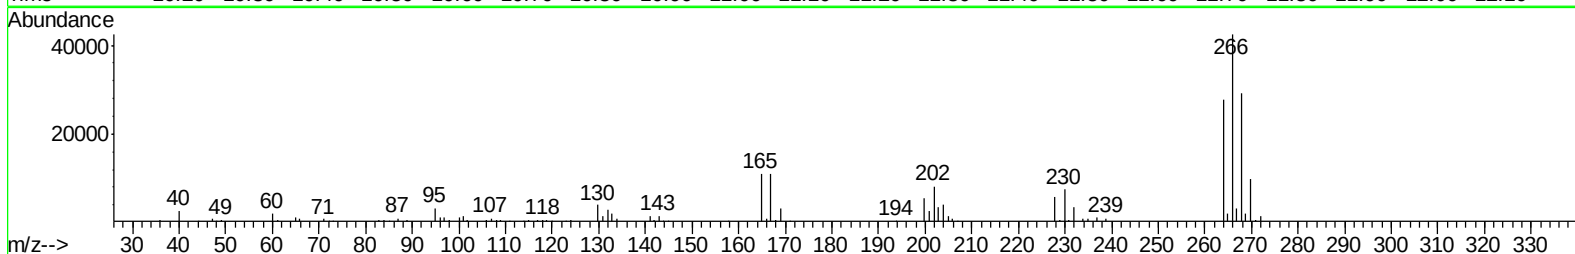


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120716\
Data File : BF091469.D
Acq On : 7 Dec 2016 15:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 07:07:22 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 08 00:35:13 2016
Response via : Initial Calibration

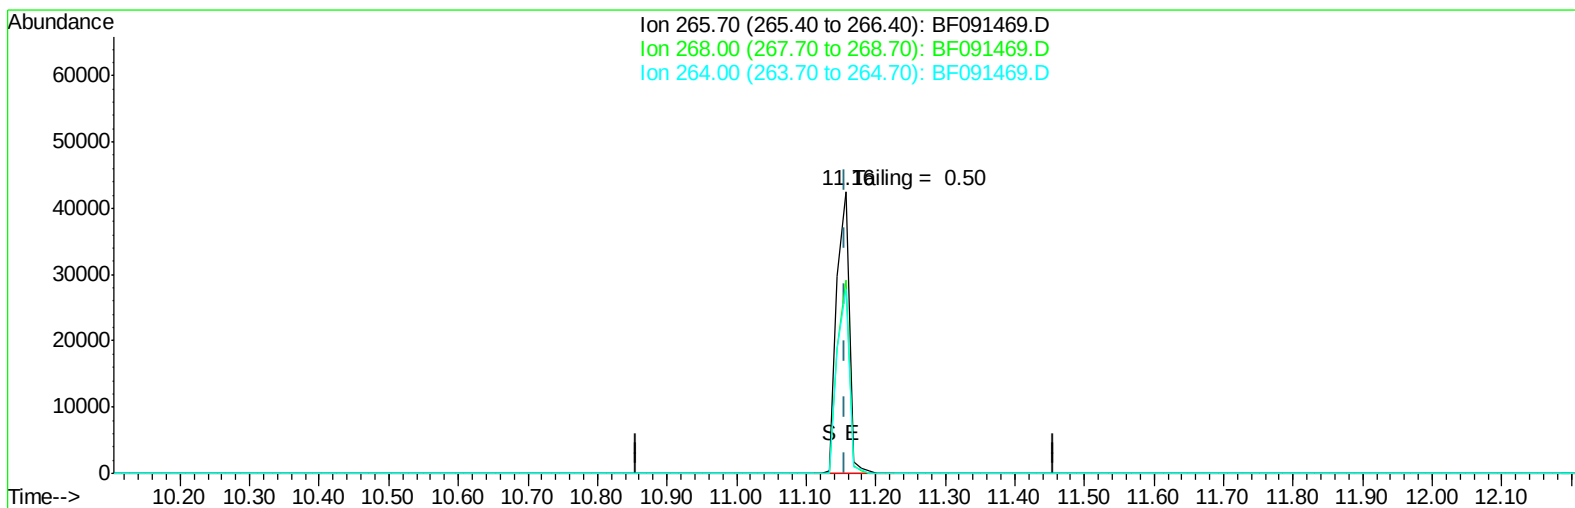

TIC: BF091469.D

(69) Pentachlorophenol (C)




11.156min (+0.000) 0.00ng

response 51778

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	68.54
264.00	60.20	65.32
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120716\  
Data File : BF091469.D  
Acq On    : 7 Dec 2016 15:02  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Dec 08 07:07:22 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 08 00:35:13 2016
Response via : Initial Calibration

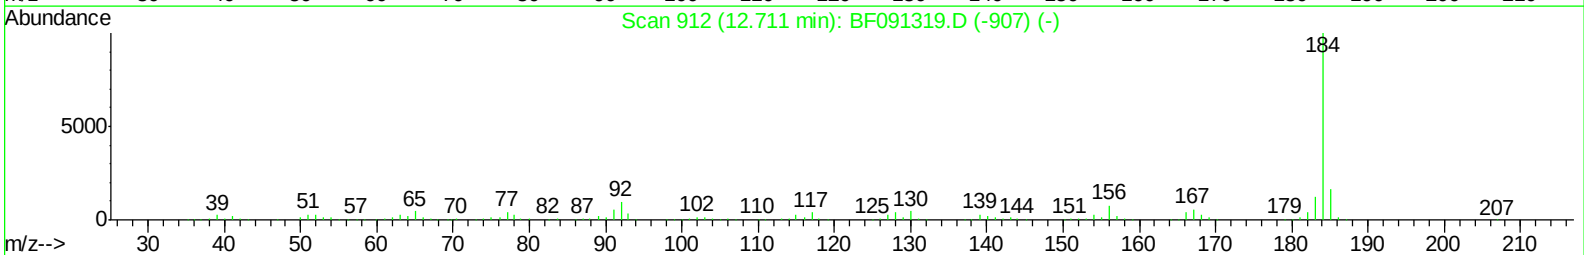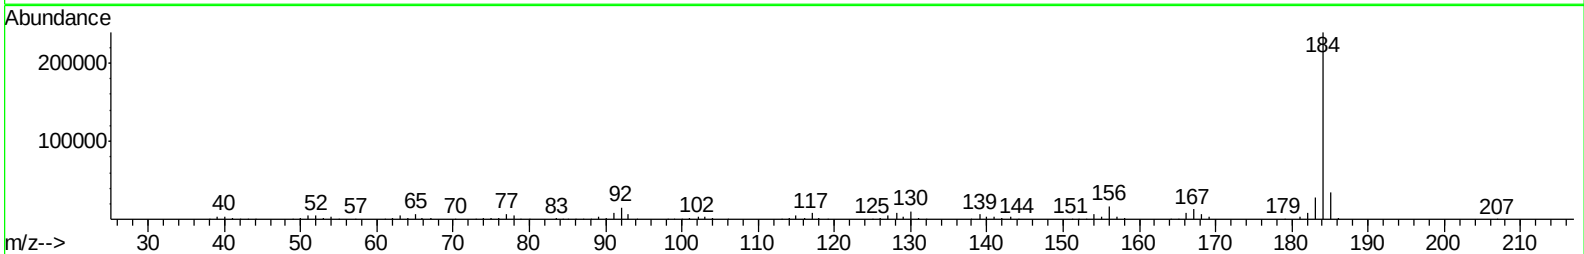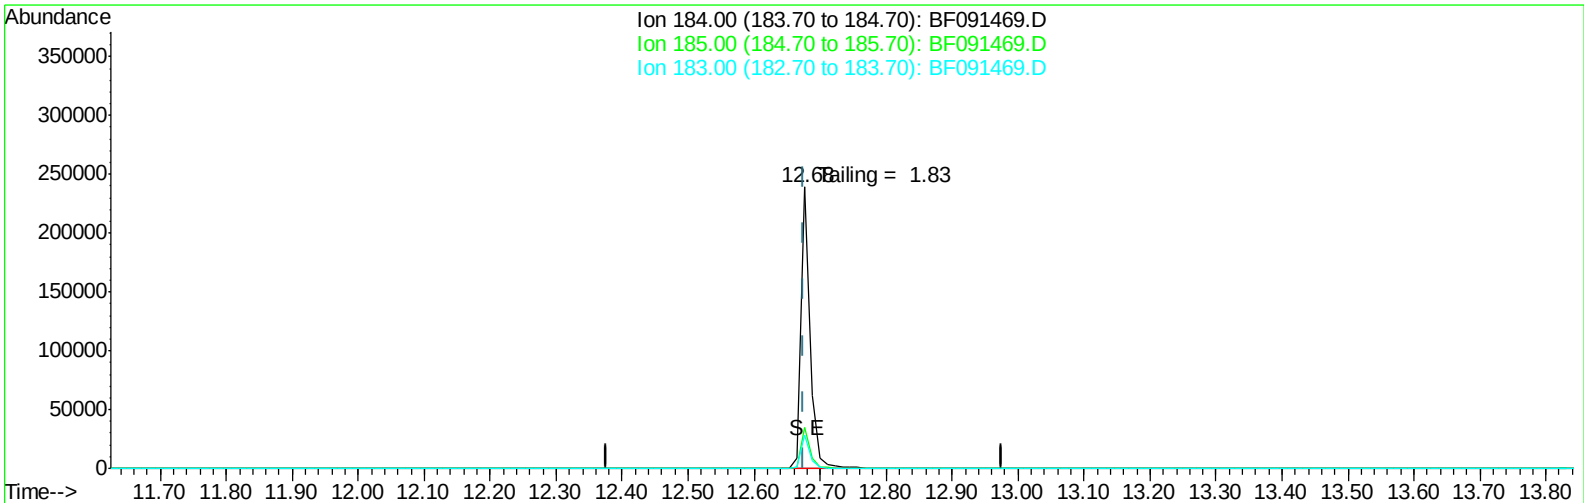

TIC: BF091469.D

(76) Benzidine

12.676min (+0.000) 0.00ng

response 226202

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	14.61
183.00	11.10	11.97
0.00	0.00	0.00