
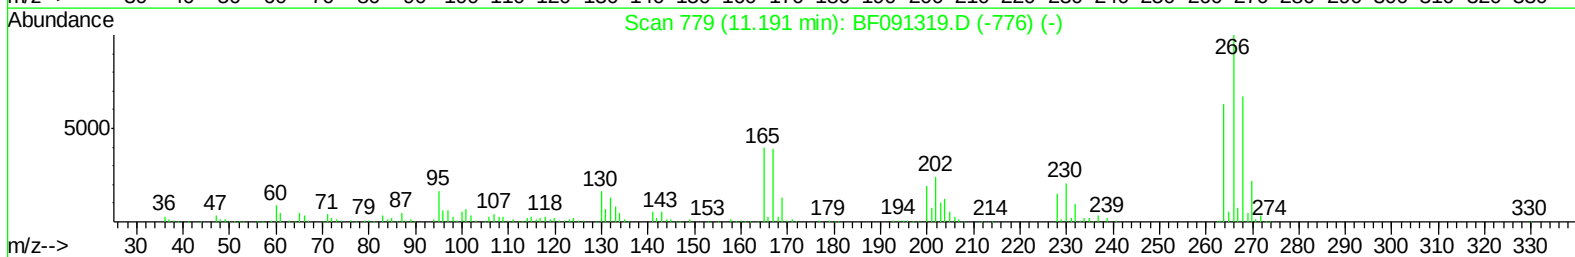
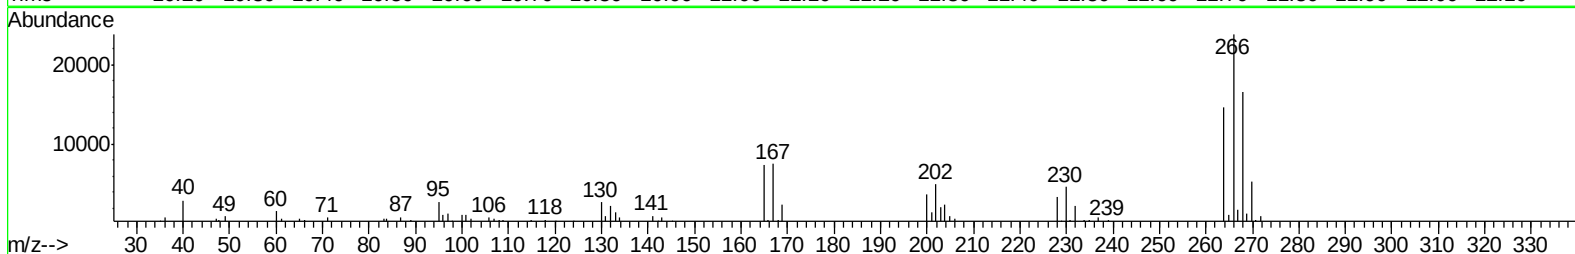


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120716\
Data File : BF091494.D
Acq On : 8 Dec 2016 3:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 07:08:15 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 08 00:35:13 2016
Response via : Initial Calibration

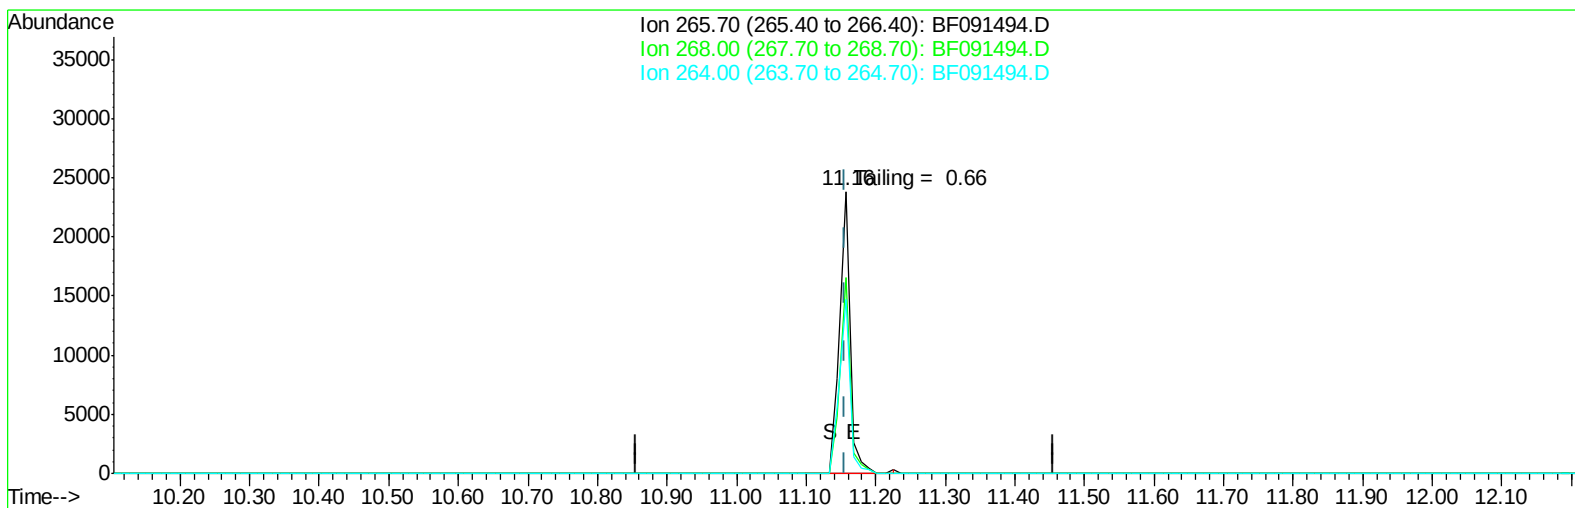

TIC: BF091494.D

(69) Pentachlorophenol (C)




11.156min (+0.000) 0.00ng

response 24543

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	69.60
264.00	60.20	61.64
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120716\
 Data File : BF091494.D
 Acq On : 8 Dec 2016 3:40
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 07:08:15 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 08 00:35:13 2016
 Response via : Initial Calibration

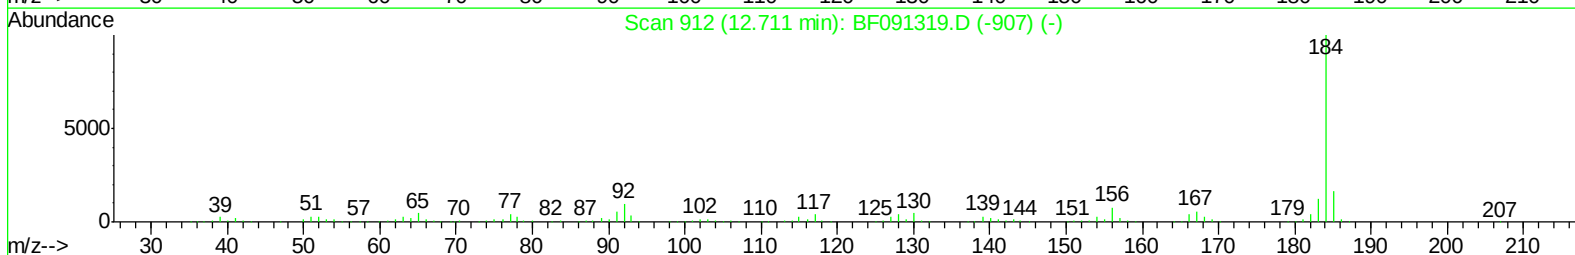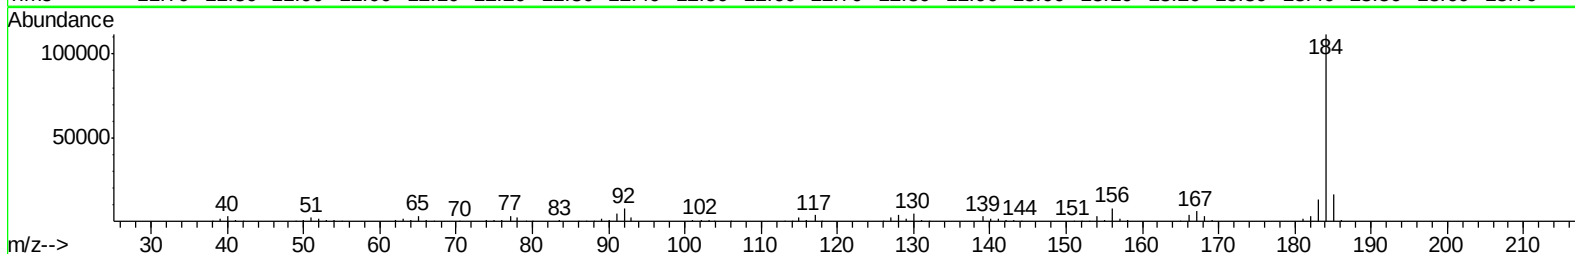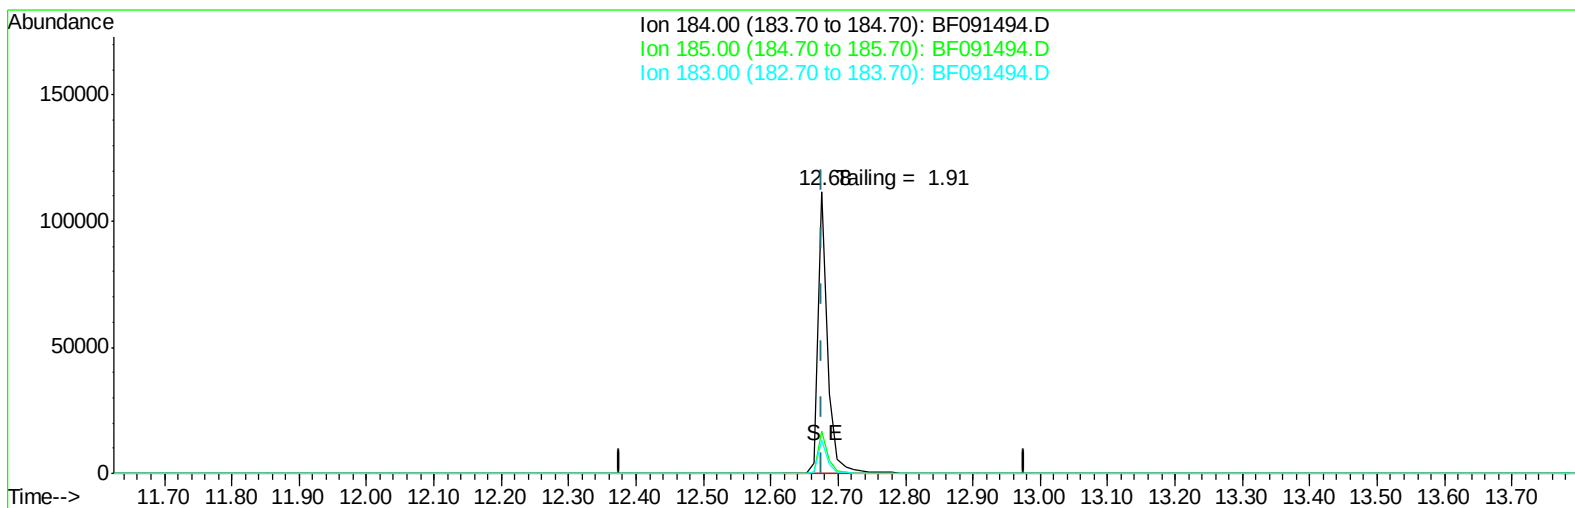

TIC: BF091494.D

(76) Benzidine

12.676min (+0.000) 0.00ng

response 109344

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	14.86
183.00	11.10	11.86
0.00	0.00	0.00