


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120716\
 Data File : BF091469.D
 Acq On : 7 Dec 2016 15:02
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 13:33:46 2016

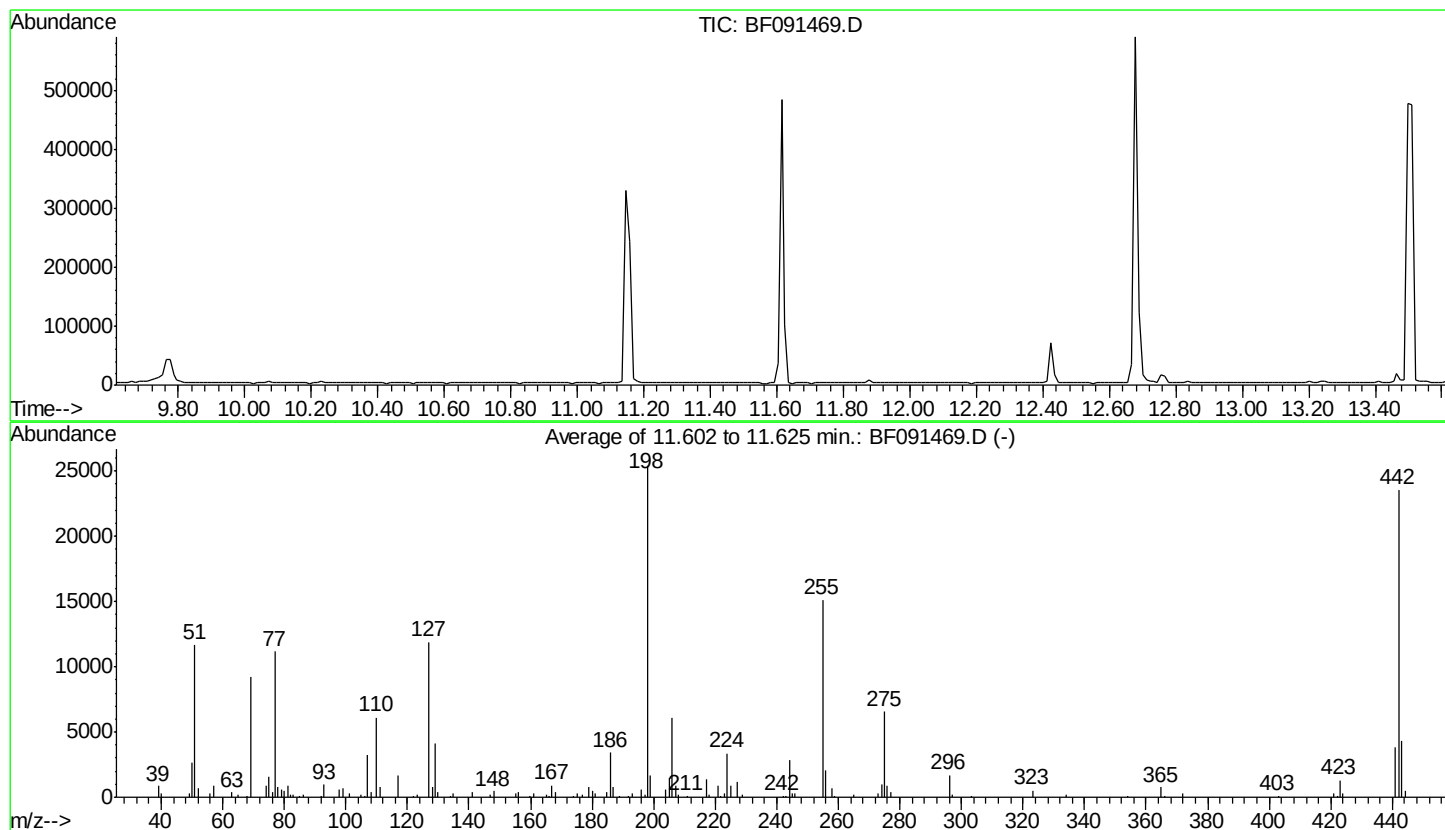

AutoFind: Scans 815, 816, 817; Background Corrected with Scan 812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	11720	PASS
68	69	0.00	2	1.5	137	PASS
69	198	0.00	100	36.1	9181	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.9	11923	PASS
197	198	0.00	2	0.9	225	PASS
198	198	100	100	100.0	25424	PASS
199	198	5	9	6.5	1659	PASS
275	198	10	60	25.8	6564	PASS
365	198	1	100	3.0	772	PASS
441	442	0.01	24	16.1	3805	PASS
442	198	50	100	92.8	23586	PASS
443	442	15	24	18.5	4365	PASS