


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120716\
 Data File : BF091494.D
 Acq On : 8 Dec 2016 3:40
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 13:33:46 2016

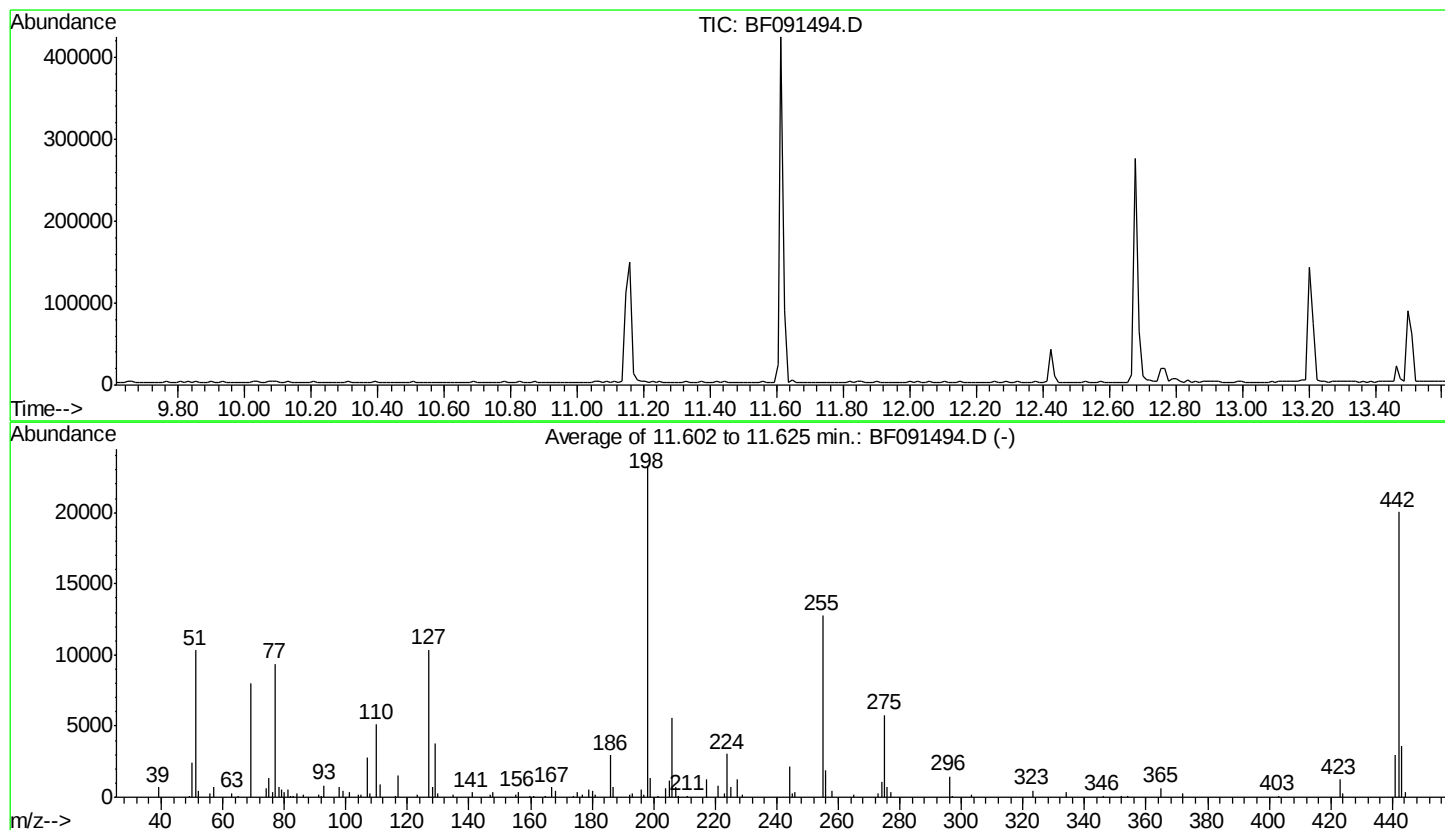

AutoFind: Scans 815, 816, 817; Background Corrected with Scan 812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	10338	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.2	7970	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.4	10347	PASS
197	198	0.00	2	0.6	149	PASS
198	198	100	100	100.0	23303	PASS
199	198	5	9	5.7	1339	PASS
275	198	10	60	24.9	5795	PASS
365	198	1	100	2.8	656	PASS
441	442	0.01	24	14.9	2975	PASS
442	198	50	100	86.0	20029	PASS
443	442	15	24	18.1	3623	PASS