
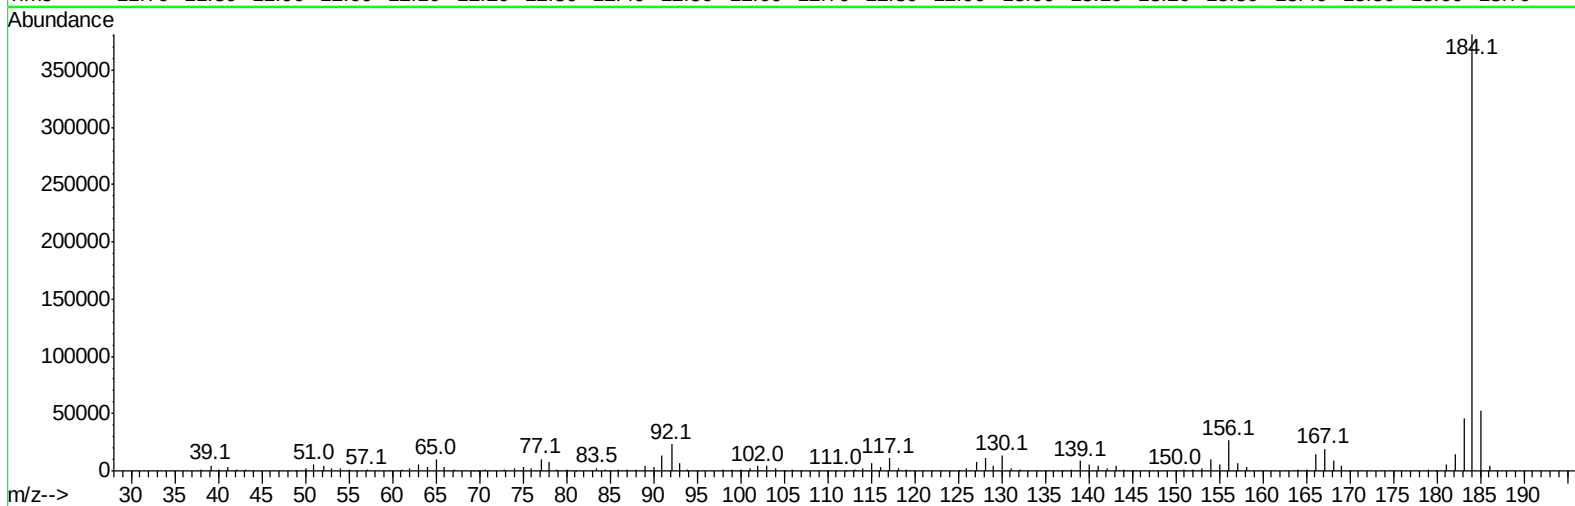


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF120717\
 Data File : BF101197.D
 Acq On : 7 Dec 2017 11:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 07:01:25 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 04 13:07:49 2017
 Response via : Initial Calibration

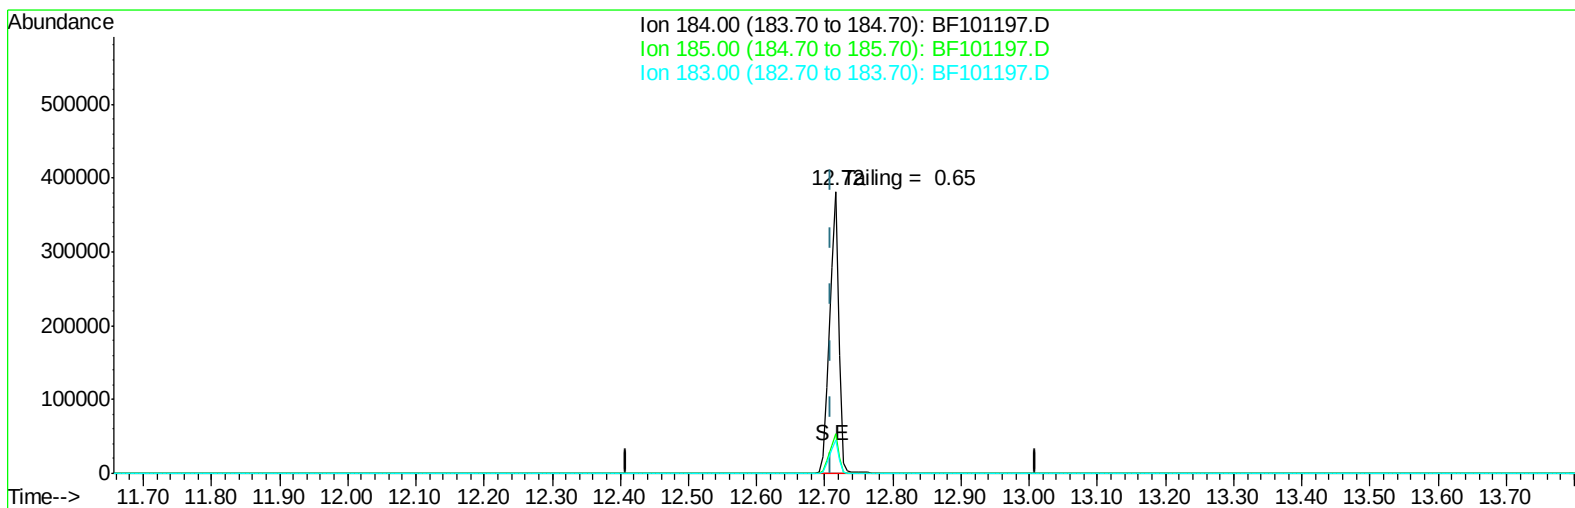

TIC: BF101197.D

(76) Benzidine



12.715min (+0.006) 0.00ng

response 349488

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.91
183.00	11.60	11.89
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF120717\
Data File : BF101197.D
Acq On : 7 Dec 2017 11:34
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 07:01:25 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 04 13:07:49 2017
Response via : Initial Calibration

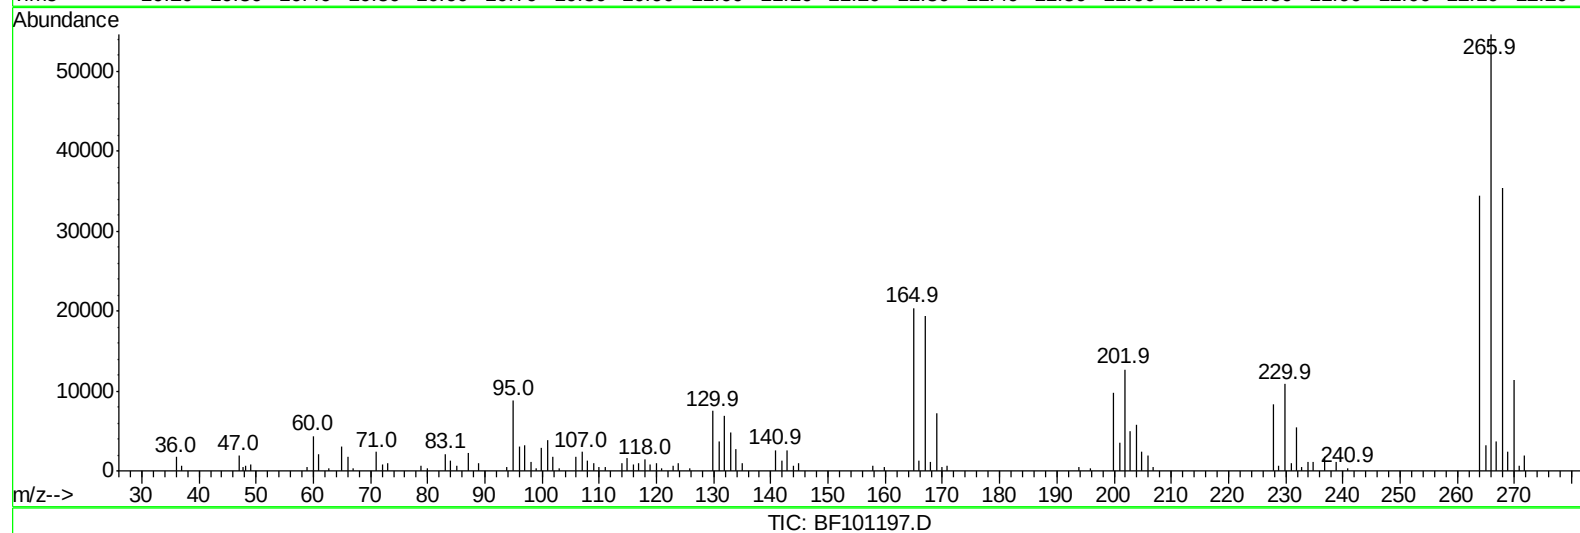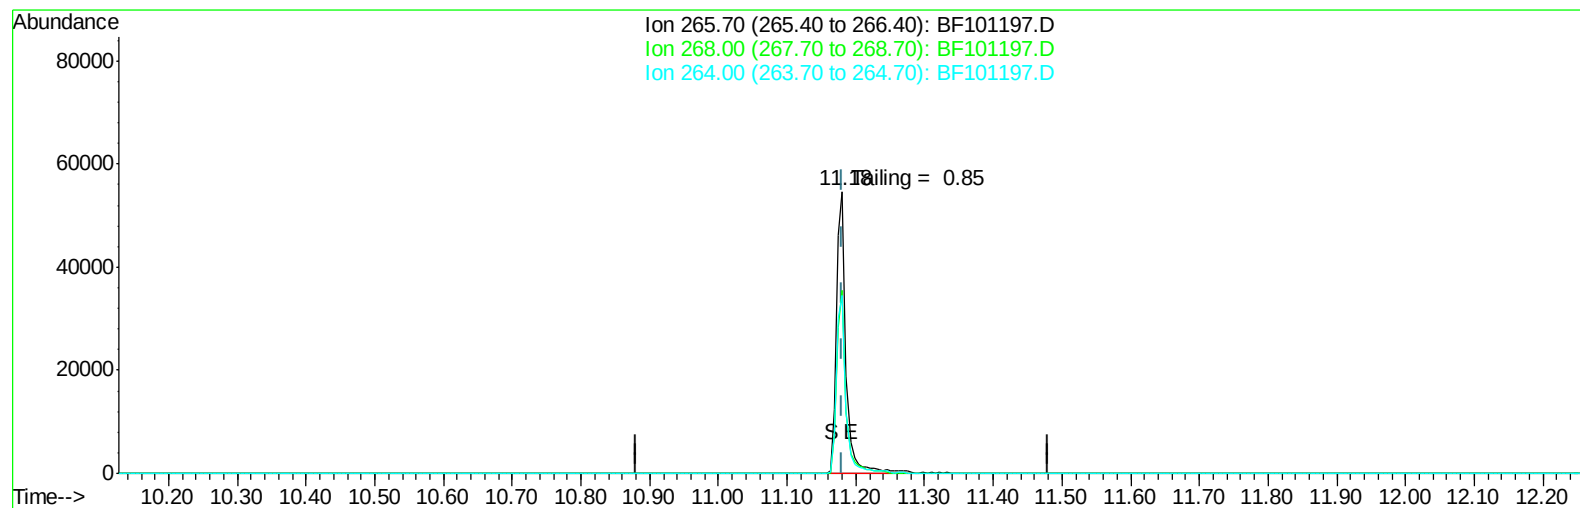

TIC: BF101197.D

(69) Pentachlorophenol (C)

11.180min (+0.000) 61614.77ng

response 53241

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.79
264.00	61.90	63.08
0.00	0.00	0.00