

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
 Data File : BF101226.D
 Acq On : 8 Dec 2017 1:38
 Operator : SJ/JU
 Sample : I6731-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 113017-TIDO-E-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	501	504	513	rBV	50333	53284	3.70%	0.674%
2	5.457	569	573	590	rVB	393499	372469	25.90%	4.711%
3	6.469	742	745	756	rVB2	270579	292079	20.31%	3.694%
4	6.610	765	769	772	rBV	895554	718898	49.98%	9.093%
5	6.839	805	808	812	rBV	316733	251615	17.49%	3.182%
6	6.998	831	835	838	rBV	1196619	1012058	70.37%	12.801%
7	7.410	900	905	908	rBV	820264	736040	51.18%	9.309%
8	8.122	1023	1026	1042	rVB	367533	303625	21.11%	3.840%
9	9.198	1205	1209	1212	rBV	1587699	1438259	100.00%	18.191%
10	9.592	1272	1276	1279	rBV	31313	25912	1.80%	0.328%
11	9.880	1322	1325	1332	rVB	358115	293339	20.40%	3.710%
12	10.298	1393	1396	1399	rVB2	19781	15128	1.05%	0.191%
13	10.674	1456	1460	1466	rBV	460223	438136	30.46%	5.542%
14	10.774	1474	1477	1486	rVB3	12653	18726	1.30%	0.237%
15	11.368	1575	1578	1582	rBV	301202	257813	17.93%	3.261%
16	12.957	1844	1848	1851	rBV	1248325	1147391	79.78%	14.512%
17	13.845	1995	1999	2007	rBV	16338	21172	1.47%	0.268%
18	14.021	2025	2029	2032	rBV	235308	228707	15.90%	2.893%
19	15.498	2275	2280	2286	rBV	140721	175173	12.18%	2.216%
20	16.303	2409	2417	2424	rVB5	11885	26878	1.87%	0.340%
21	16.998	2527	2535	2544	rVB7	15857	38623	2.69%	0.489%
22	17.839	2669	2678	2686	rBV5	13875	41056	2.85%	0.519%


Sum of corrected areas: 7906381

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120717\
Data File : BF101226.D
Acq On : 8 Dec 2017 1:38
Operator : SJ/JU
Sample : I6731-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
113017-TIDO-E-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

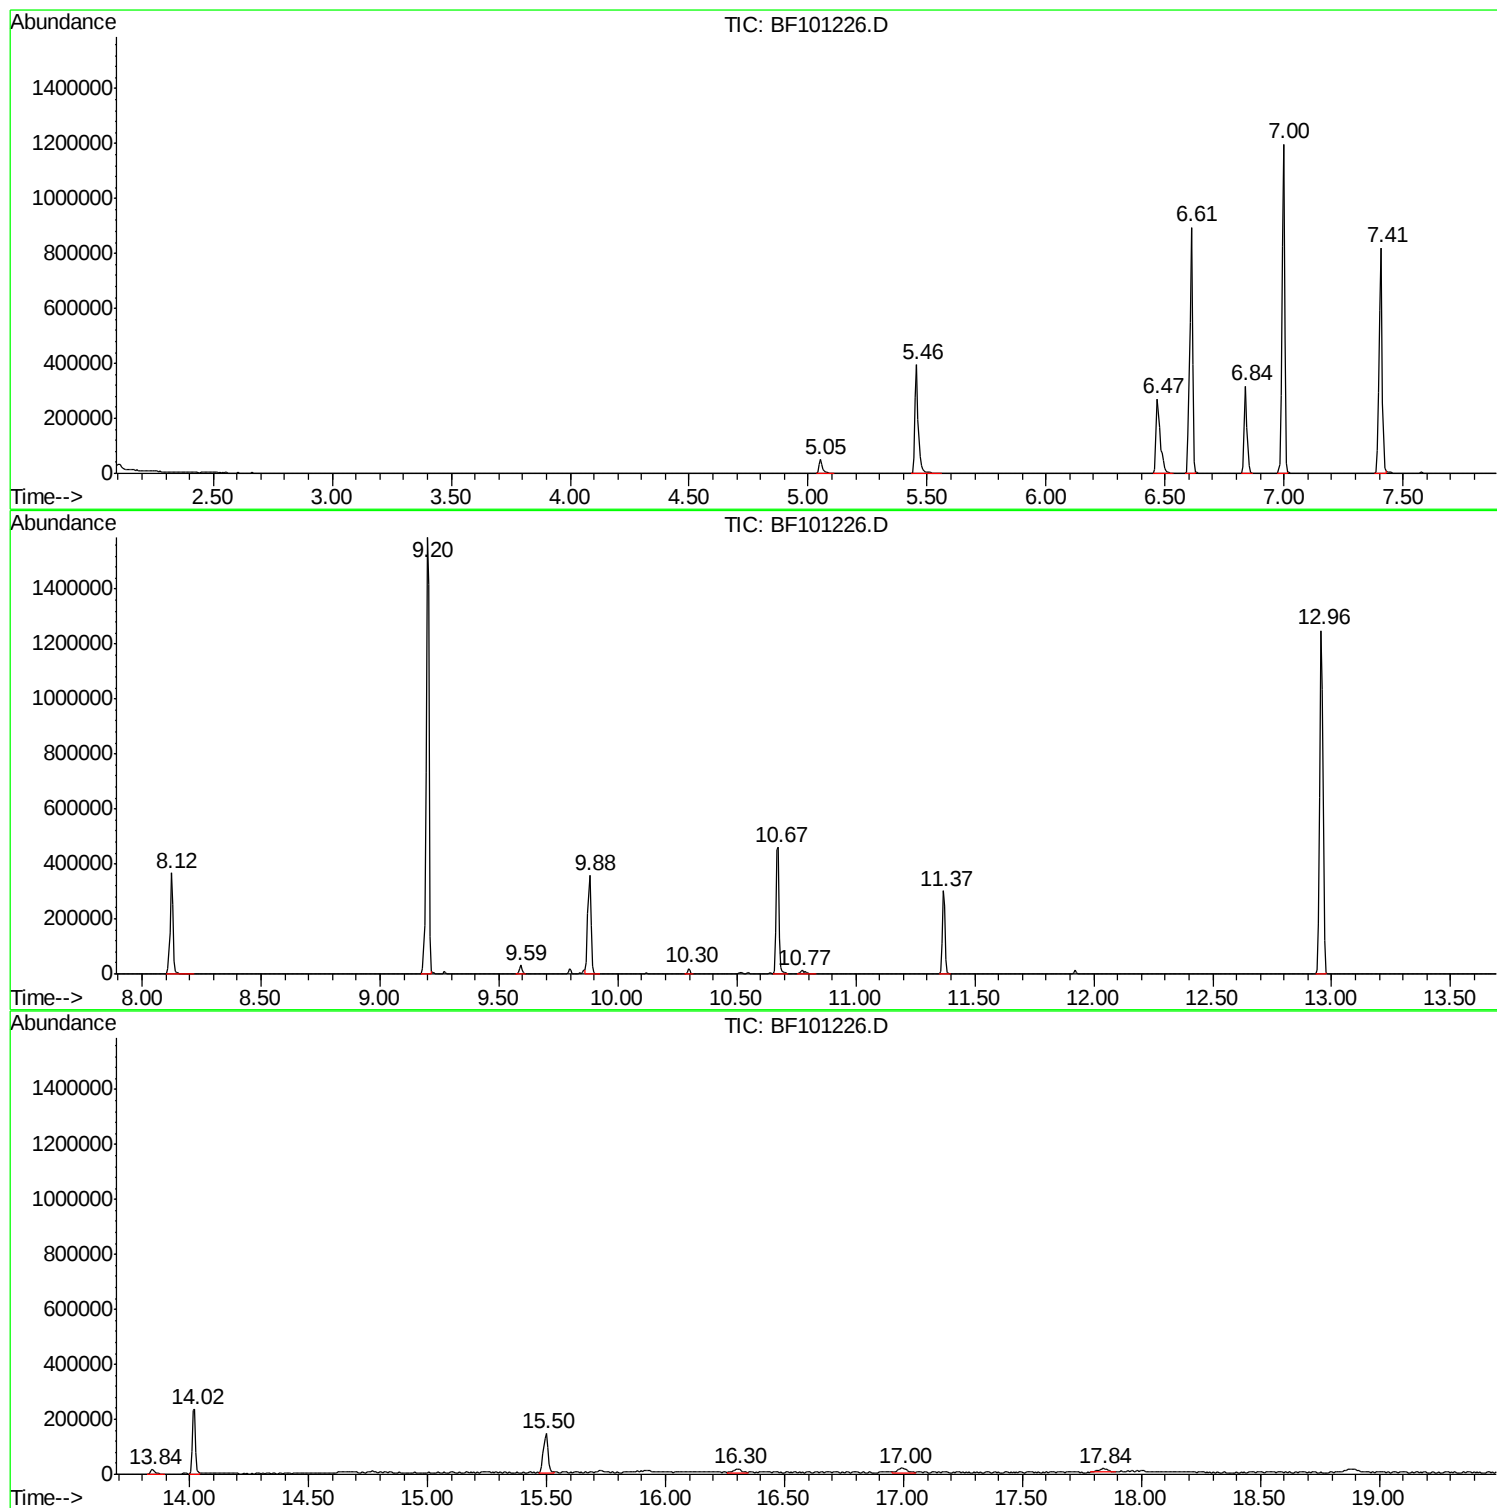

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
Data_File : BF101226.D
Acq_On : 8_Dec_2017. 1:388
Operator : SJ/JUU
Sample : I6731-033
Misc :
ALS_Vial : 28 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
113017-TIDO-E-U-B

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
