

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
 Data File : BF101227.D
 Acq On : 8 Dec 2017 2:05
 Operator : SJ/JU
 Sample : I6731-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 113017-TIDO-E-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	501	504	512	rBV	48624	53110	3.99%	0.728%
2	5.457	570	573	586	rBV	397230	365640	27.45%	5.009%
3	6.469	742	745	760	rVB2	246244	260477	19.56%	3.568%
4	6.610	765	769	772	rBV	832156	674910	50.67%	9.246%
5	6.839	805	808	814	rBB	322066	249971	18.77%	3.425%
6	6.998	831	835	838	rBV	1126367	948839	71.24%	12.999%
7	7.410	900	905	908	rBV	734375	687741	51.64%	9.422%
8	8.122	1023	1026	1038	rVB	358230	297128	22.31%	4.071%
9	9.198	1205	1209	1212	rBV	1449335	1331892	100.00%	18.247%
10	9.798	1308	1311	1315	rBB	18557	14159	1.06%	0.194%
11	9.880	1319	1325	1331	rVB	344341	295708	22.20%	4.051%
12	10.298	1393	1396	1399	rBB2	20937	15343	1.15%	0.210%
13	10.674	1456	1460	1469	rBB	422710	394073	29.59%	5.399%
14	10.774	1473	1477	1482	rBV2	11348	14396	1.08%	0.197%
15	11.368	1575	1578	1582	rBV	290089	251402	18.88%	3.444%
16	12.957	1844	1848	1851	rBV	1141722	1051071	78.92%	14.399%
17	14.021	2025	2029	2032	rBV	245994	224544	16.86%	3.076%
18	15.498	2275	2280	2290	rVB	136134	168985	12.69%	2.315%


Sum of corrected areas: 7299389

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120717\
Data File : BF101227.D
Acq On : 8 Dec 2017 2:05
Operator : SJ/JU
Sample : I6731-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
113017-TIDO-E-U-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

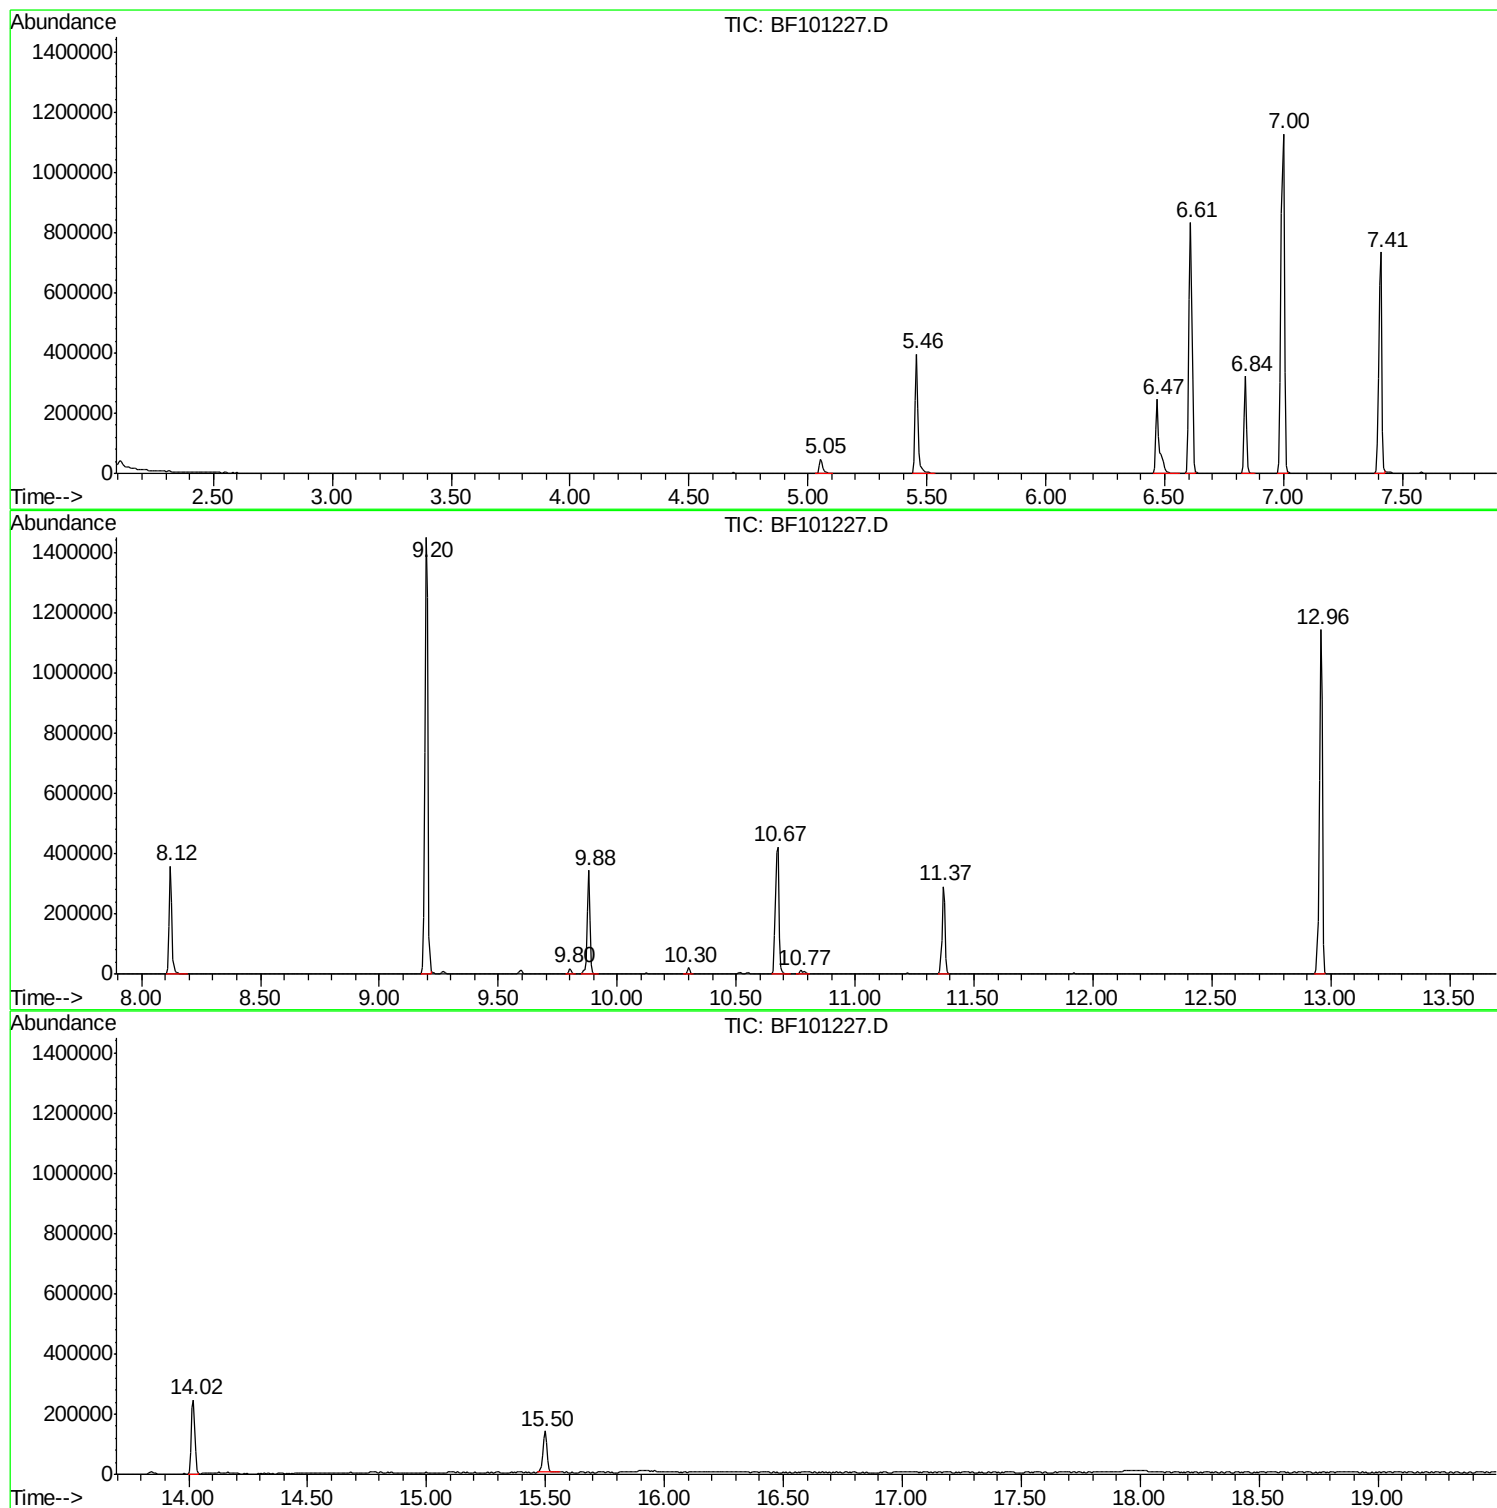

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
Data_File : BF101227.D
Acq_On : 8-Dec-2017 2:055
Operator : SJ/JUU
Sample : I6731-044
Misc :
ALS_Vial : 29 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
113017-TIDO-E-U-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
