

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
 Data File : BF101229.D
 Acq On : 8 Dec 2017 2:59
 Operator : SJ/JU
 Sample : I6732-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120117-TIDO-F-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	501	504	515	rBV	48168	54678	4.06%	0.744%
2	5.457	569	573	586	rBV	394816	375080	27.88%	5.101%
3	6.469	742	745	758	rVB2	256663	279659	20.79%	3.803%
4	6.610	765	769	772	rBV	867314	688088	51.15%	9.358%
5	6.839	805	808	815	rBB	291811	228185	16.96%	3.103%
6	6.998	831	835	838	rBV	1150708	966496	71.84%	13.144%
7	7.410	900	905	908	rBV	747544	689635	51.26%	9.379%
8	8.122	1023	1026	1031	rBV	338525	270237	20.09%	3.675%
9	9.198	1205	1209	1212	rBV	1509502	1345364	100.00%	18.297%
10	9.592	1271	1276	1278	rBV	22031	17093	1.27%	0.232%
11	9.880	1319	1325	1330	rVB2	311208	272591	20.26%	3.707%
12	10.298	1393	1396	1399	rVB2	22790	17526	1.30%	0.238%
13	10.669	1456	1459	1469	rBB	442240	405708	30.16%	5.518%
14	10.769	1474	1476	1484	rBB2	12495	16292	1.21%	0.222%
15	11.369	1575	1578	1583	rBV	288847	233600	17.36%	3.177%
16	12.957	1844	1848	1851	rBV	1160780	1082965	80.50%	14.728%
17	13.839	1995	1998	2005	rBV2	30774	35479	2.64%	0.483%
18	14.015	2025	2028	2032	rBV	223395	210181	15.62%	2.858%
19	15.498	2274	2280	2287	rVB	129816	164235	12.21%	2.234%


Sum of corrected areas: 7353092

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
Data File : BF101229.D
Acq On : 8 Dec 2017 2:59
Operator : SJ/JU
Sample : I6732-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120117-TIDO-F-D-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

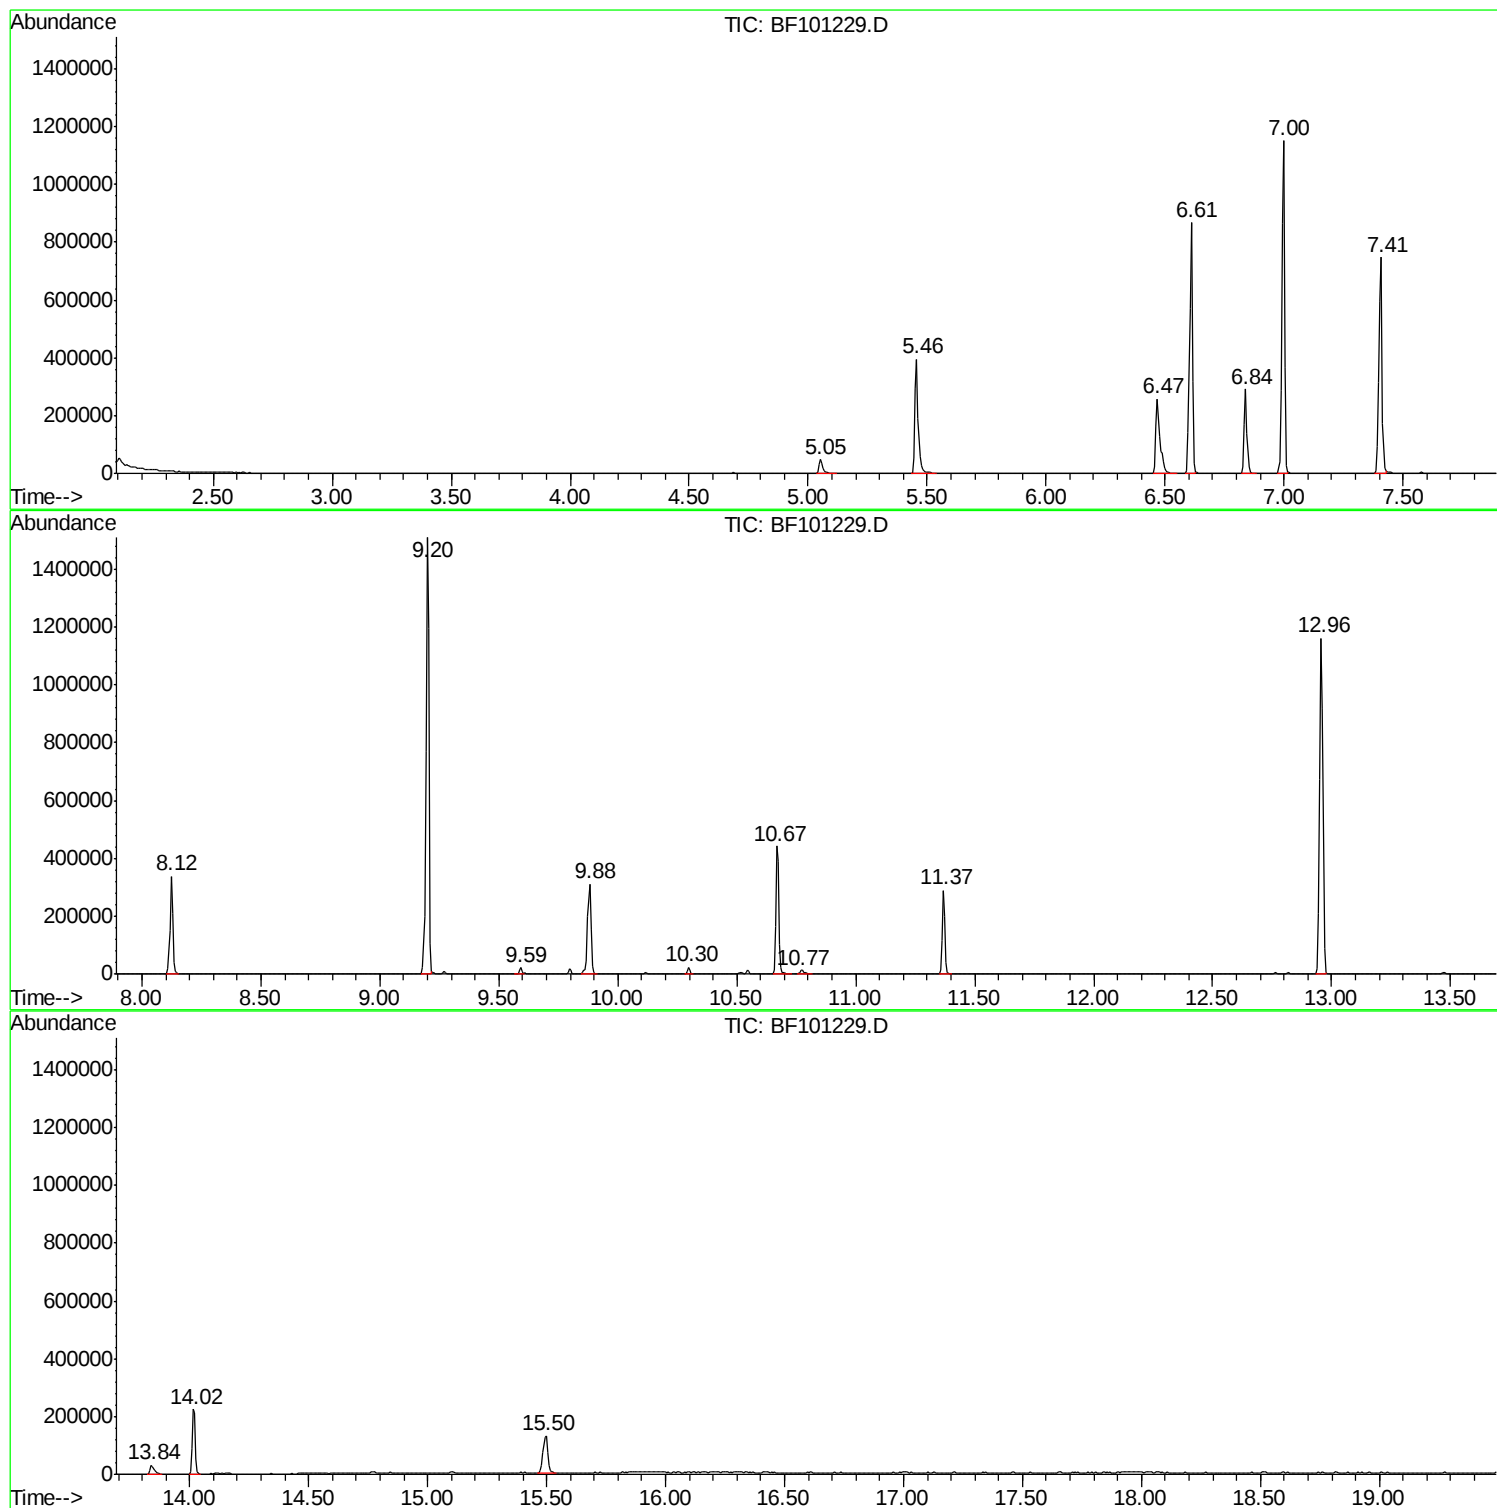

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
Data_File : BF101229.D
Acq_On : 8-Dec-2017 2:599
Operator : SJ/JUU
Sample : I6732-022
Misc :
ALS_Vial : 31 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120117-TIDO-F-D-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
