

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
 Data File : BF101231.D
 Acq On : 8 Dec 2017 3:53
 Operator : SJ/JU
 Sample : I6732-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120117-TIDO-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	501	504	510	rBV	38292	42653	3.31%	0.588%
2	5.457	569	573	586	rBV	332921	350360	27.20%	4.827%
3	6.469	742	745	759	rVB2	233486	255950	19.87%	3.526%
4	6.610	765	769	772	rBV	803006	655401	50.88%	9.029%
5	6.840	805	808	814	rBB	294728	232088	18.02%	3.197%
6	6.998	830	835	838	rBV	1077294	933372	72.46%	12.859%
7	7.410	900	905	908	rBV	683435	653588	50.74%	9.004%
8	8.122	1022	1026	1040	rBV	338957	274503	21.31%	3.782%
9	9.198	1205	1209	1212	rBV	1547409	1288098	100.00%	17.746%
10	9.881	1319	1325	1330	rVB	319468	269974	20.96%	3.719%
11	10.669	1456	1459	1468	rBB	428287	382027	29.66%	5.263%
12	11.369	1574	1578	1582	rBV	297613	235010	18.24%	3.238%
13	12.957	1844	1848	1851	rBV	1152638	1000093	77.64%	13.778%
14	14.016	2024	2028	2032	rBV	223673	205103	15.92%	2.826%
15	15.498	2273	2280	2284	rBV	128052	160930	12.49%	2.217%
16	15.727	2313	2319	2326	rVB2	14798	25411	1.97%	0.350%
17	16.304	2410	2417	2422	rBV4	21547	41247	3.20%	0.568%
18	16.992	2527	2534	2546	rVB3	29784	78239	6.07%	1.078%
19	17.833	2668	2677	2687	rBV3	27741	85990	6.68%	1.185%
20	18.868	2844	2853	2866	rVB7	23750	88565	6.88%	1.220%




Sum of corrected areas: 7258602

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
Data File : BF101231.D
Acq On : 8 Dec 2017 3:53
Operator : SJ/JU
Sample : I6732-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120117-TIDO-F-U-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

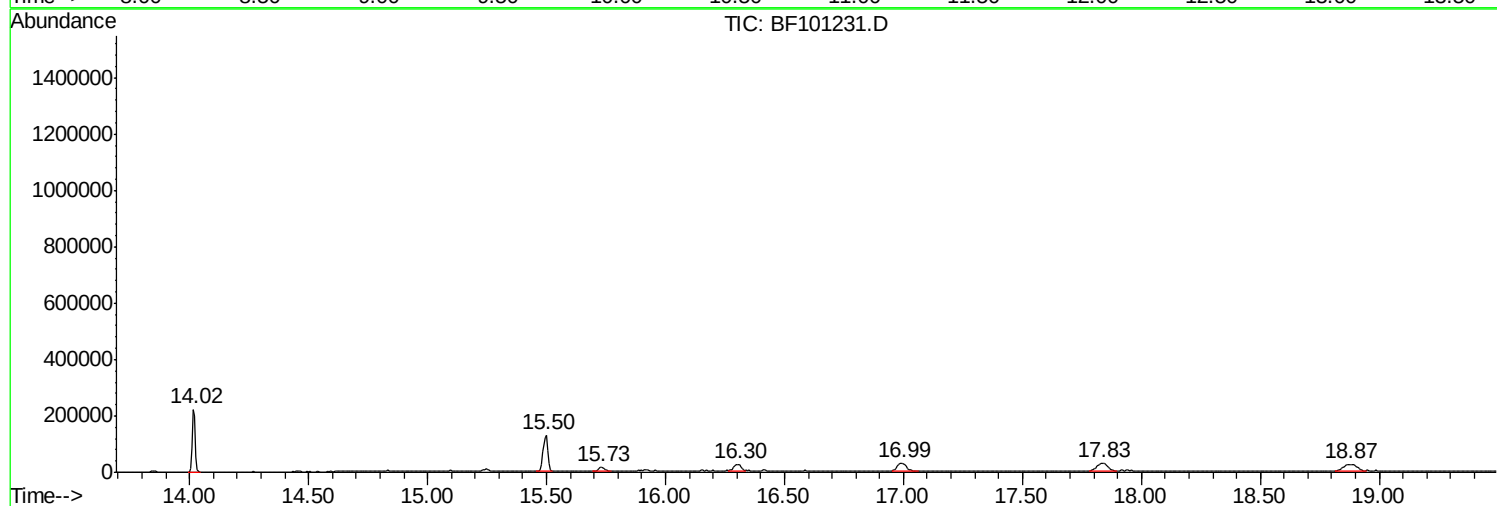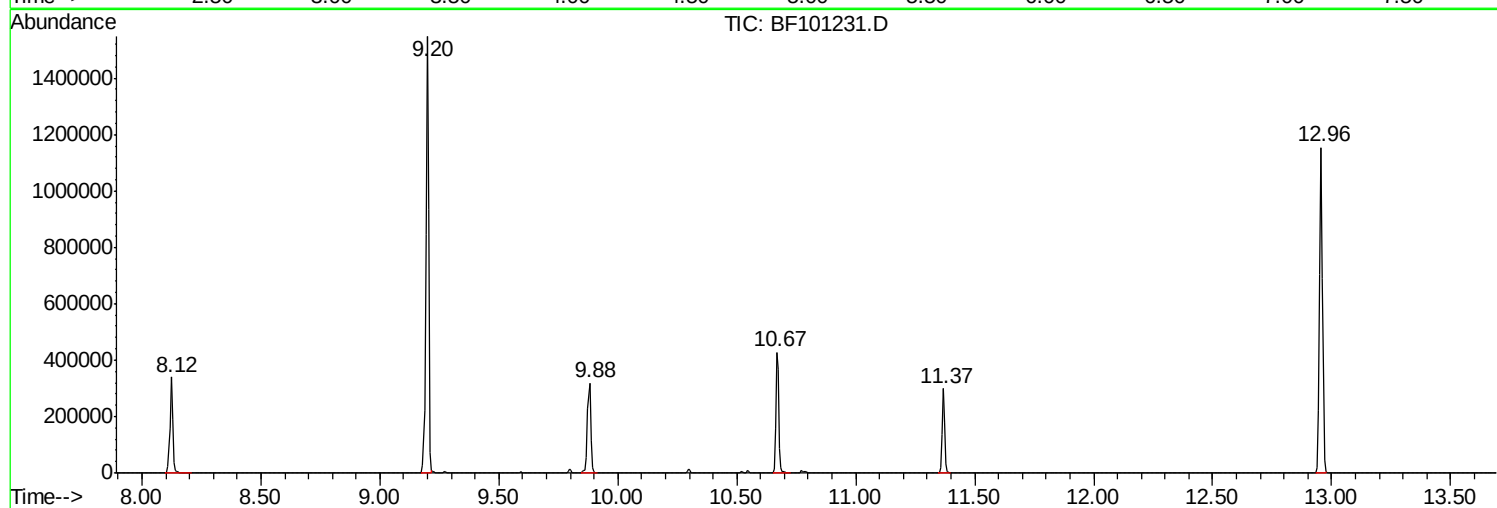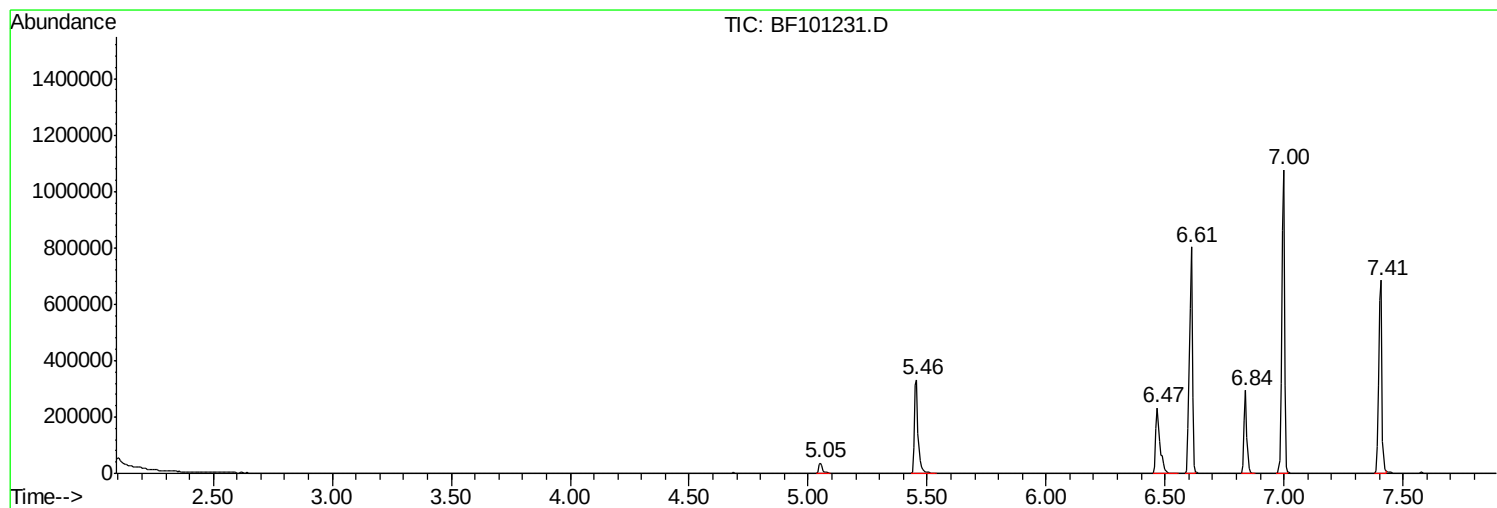

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
Data_File : BF101231.D
Acq_On : 8_Dec_2017. 3:533
Operator : SJ/JUU
Sample : I6732-044
Misc :
ALS_Vial : 33 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120117-TIDO-F-U-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
