

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
 Data File : BF101232.D
 Acq On : 8 Dec 2017 4:20
 Operator : SJ/JU
 Sample : I6732-05
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120117-FOPI-E-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	501	504	511	rBV	40352	47667	3.90%	0.700%
2	5.457	569	573	591	rVB	305666	328123	26.83%	4.821%
3	6.469	742	745	756	rBV2	206893	234214	19.15%	3.441%
4	6.610	765	769	772	rBV	753577	617739	50.52%	9.076%
5	6.839	805	808	812	rBV	299712	234292	19.16%	3.442%
6	6.998	831	835	838	rBV	1006940	881321	72.07%	12.948%
7	7.410	900	905	908	rBV	634004	620007	50.70%	9.109%
8	8.122	1023	1026	1038	rVB	342807	278330	22.76%	4.089%
9	9.198	1205	1209	1212	rBV	1484567	1222860	100.00%	17.966%
10	9.880	1319	1325	1328	rBV	313983	269945	22.07%	3.966%
11	10.669	1456	1459	1469	rBB	401004	359969	29.44%	5.289%
12	11.368	1575	1578	1582	rBV	284208	235865	19.29%	3.465%
13	12.957	1844	1848	1851	rBV	1136018	985293	80.57%	14.476%
14	13.845	1995	1999	2006	rBV	19284	23579	1.93%	0.346%
15	14.015	2025	2028	2032	rBV	243016	217227	17.76%	3.192%
16	14.115	2032	2045	2058	rVB4	11248	51396	4.20%	0.755%
17	15.498	2274	2280	2285	rBV	131316	170212	13.92%	2.501%
18	15.915	2349	2351	2364	rVB6	13348	28342	2.32%	0.416%


Sum of corrected areas: 6806381

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120717\
Data File : BF101232.D
Acq On : 8 Dec 2017 4:20
Operator : SJ/JU
Sample : I6732-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120117-FOPI-E-D-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

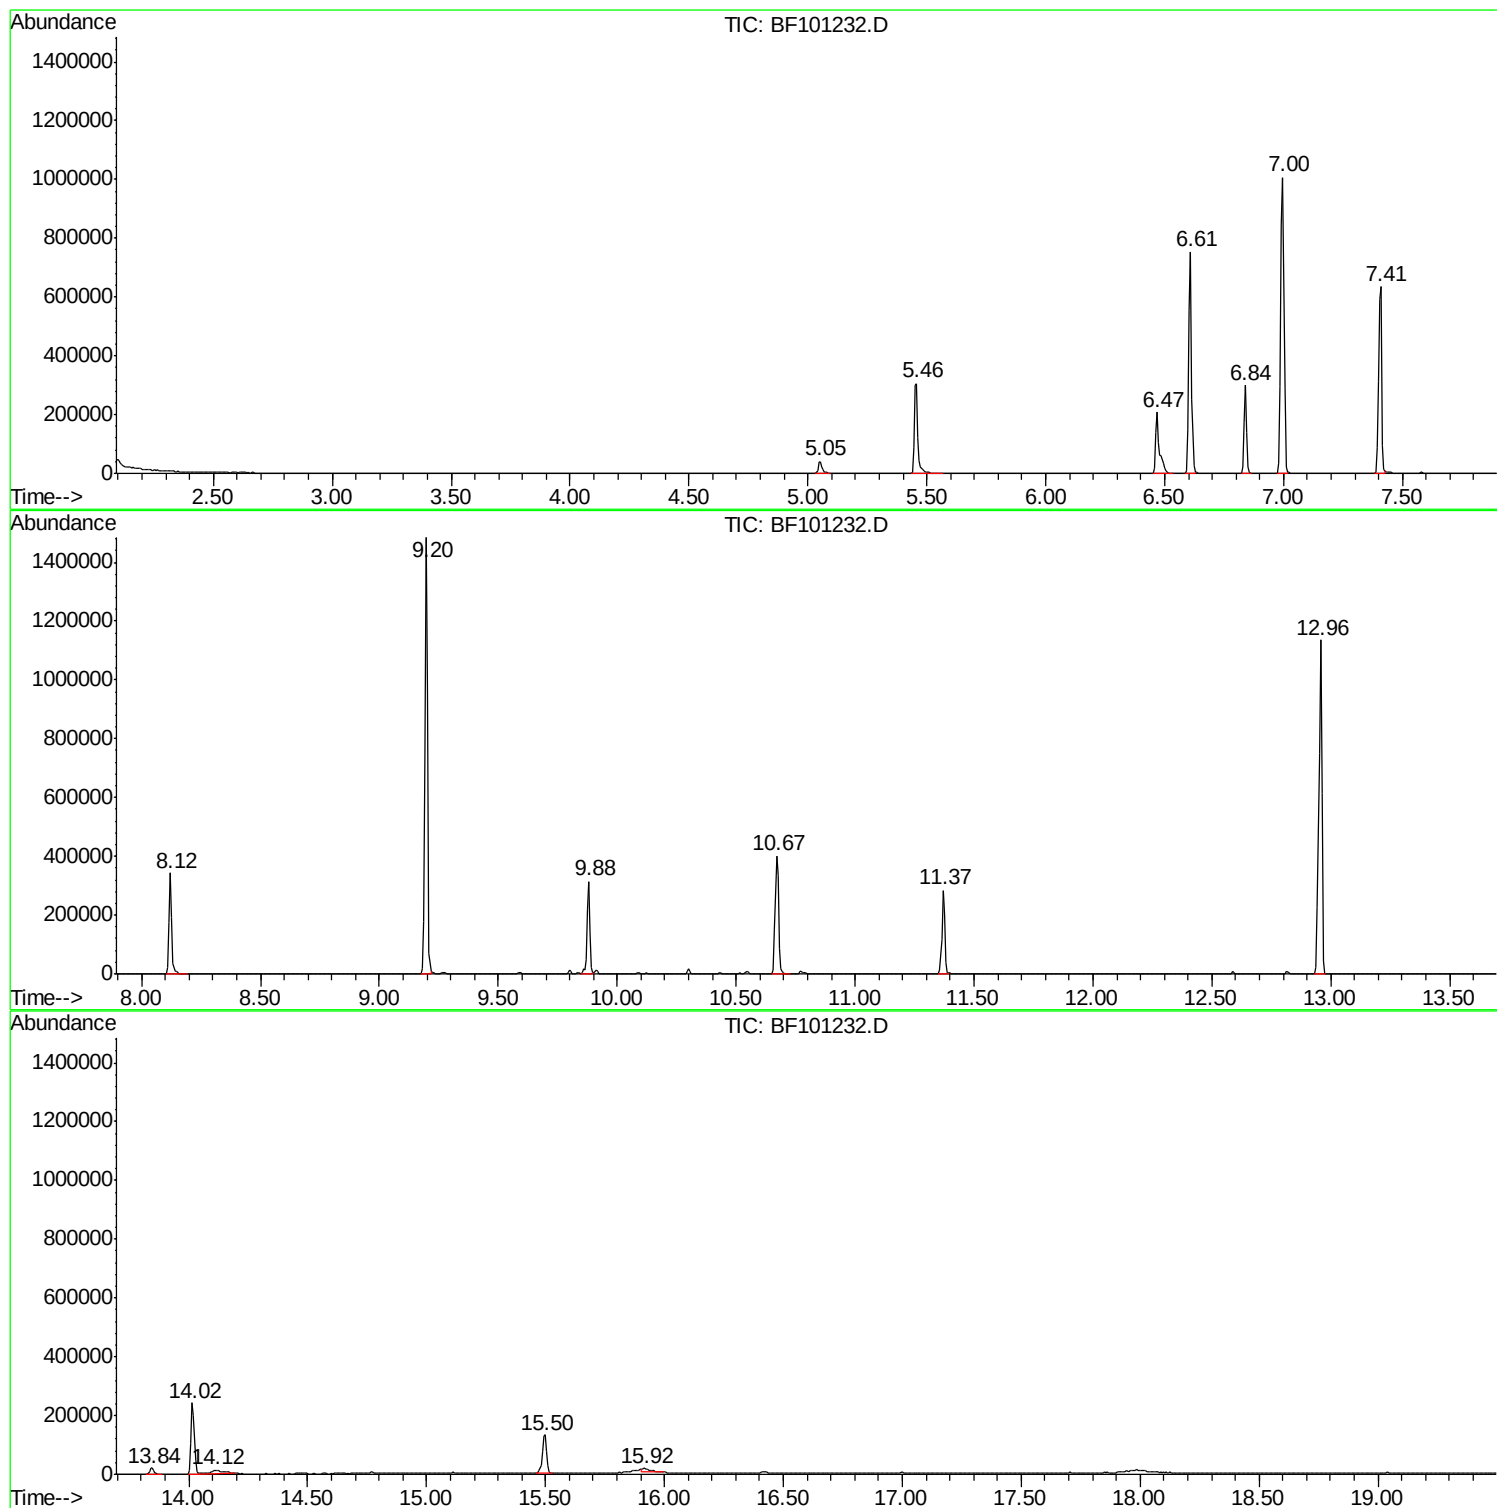

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF120717\
Data_File : BF101232.D
Acq_On : 8_Dec_2017. 4:200
Operator : SJ/JUU
Sample : I6732-055
Misc :
ALS_Vial : 34 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120117-FOPI-E-D-M

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
