


Data Path : Z:\HPCHEM1\BNA F\Data\BF120717\
 Data File : BF101197.D
 Acq On : 7 Dec 2017 11:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 04 13:07:49 2017

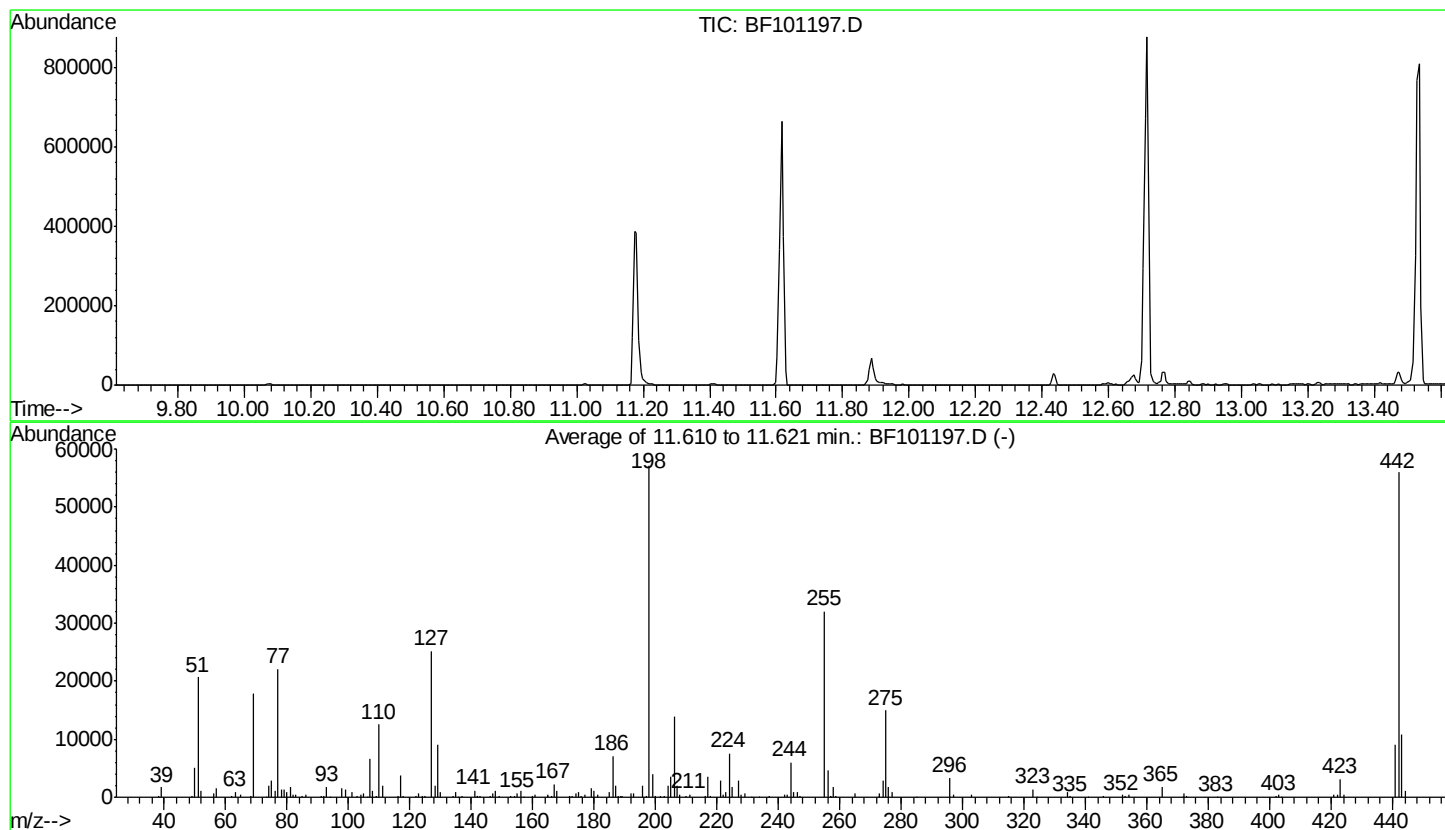

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	20661	PASS
68	69	0.00	2	1.8	317	PASS
69	198	0.00	100	31.5	17987	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	25237	PASS
197	198	0.00	2	0.3	151	PASS
198	198	100	100	100.0	57157	PASS
199	198	5	9	6.9	3924	PASS
275	198	10	60	26.1	14905	PASS
365	198	1	100	3.2	1812	PASS
441	443	0.01	100	85.1	9116	PASS
442	198	50	100	98.1	56053	PASS
443	442	15	24	19.1	10708	PASS