
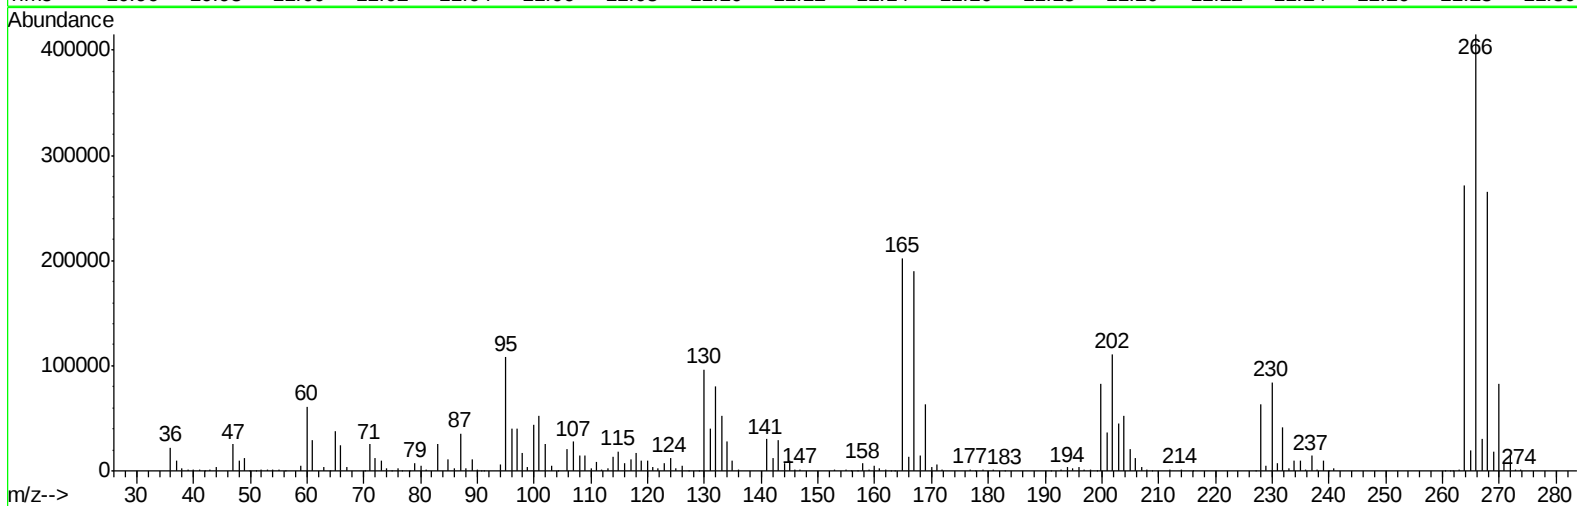


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120718\
Data File : BF111177.D
Acq On : 7 Dec 2018 10:44
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 05:41:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 05 17:30:55 2018
Response via : Initial Calibration

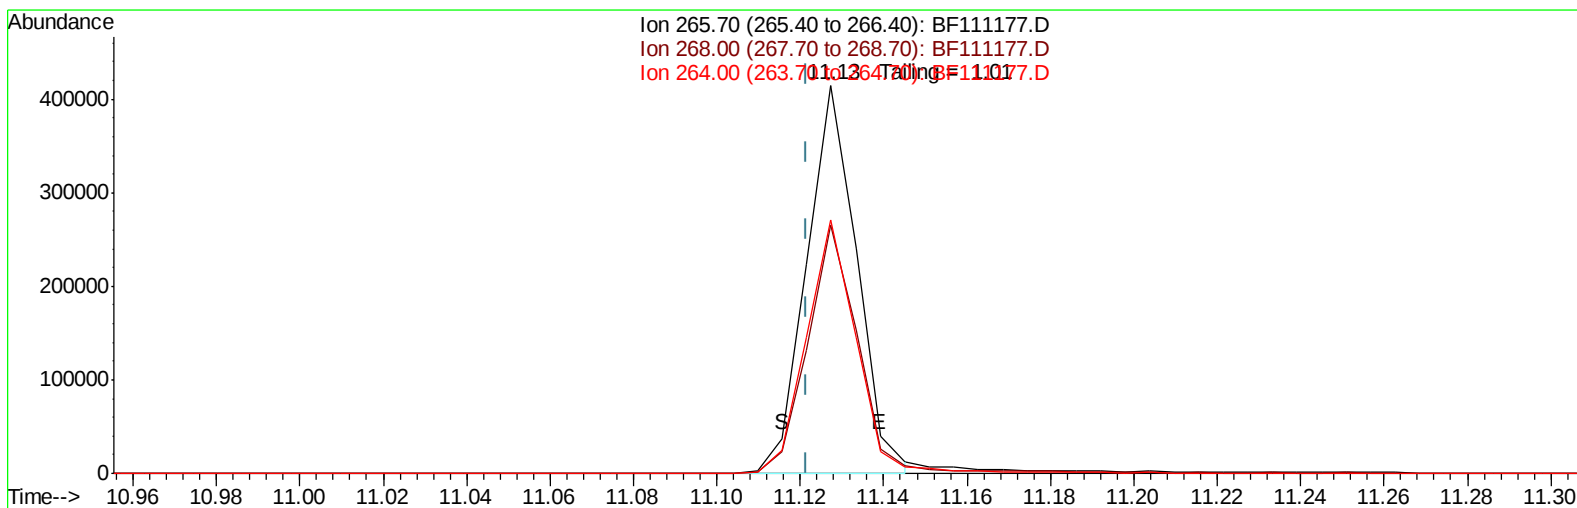

TIC: BF111177.D

(70) Pentachlorophenol (C)



11.127min (+0.006) 145432.60ng

response 354036

Ion	Exp%	Act%
265.70	100	100
268.00	65.30	63.92
264.00	63.50	65.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120718\
 Data File : BF111177.D
 Acq On : 7 Dec 2018 10:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 05:41:06 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 05 17:30:55 2018
 Response via : Initial Calibration

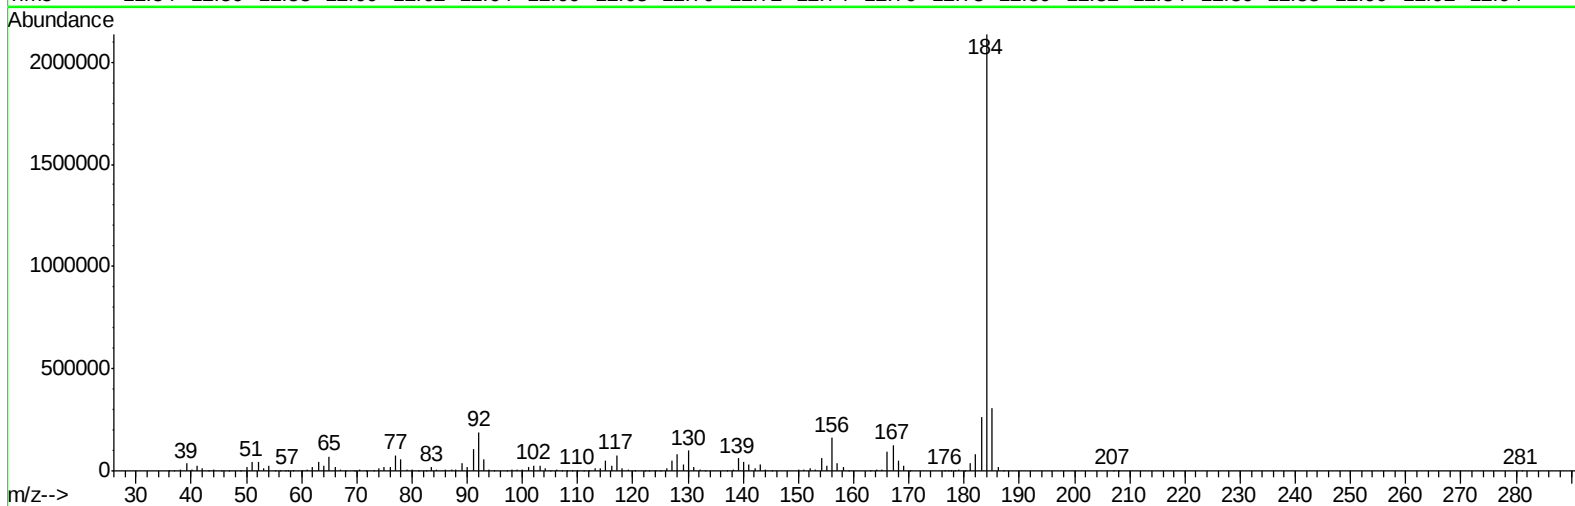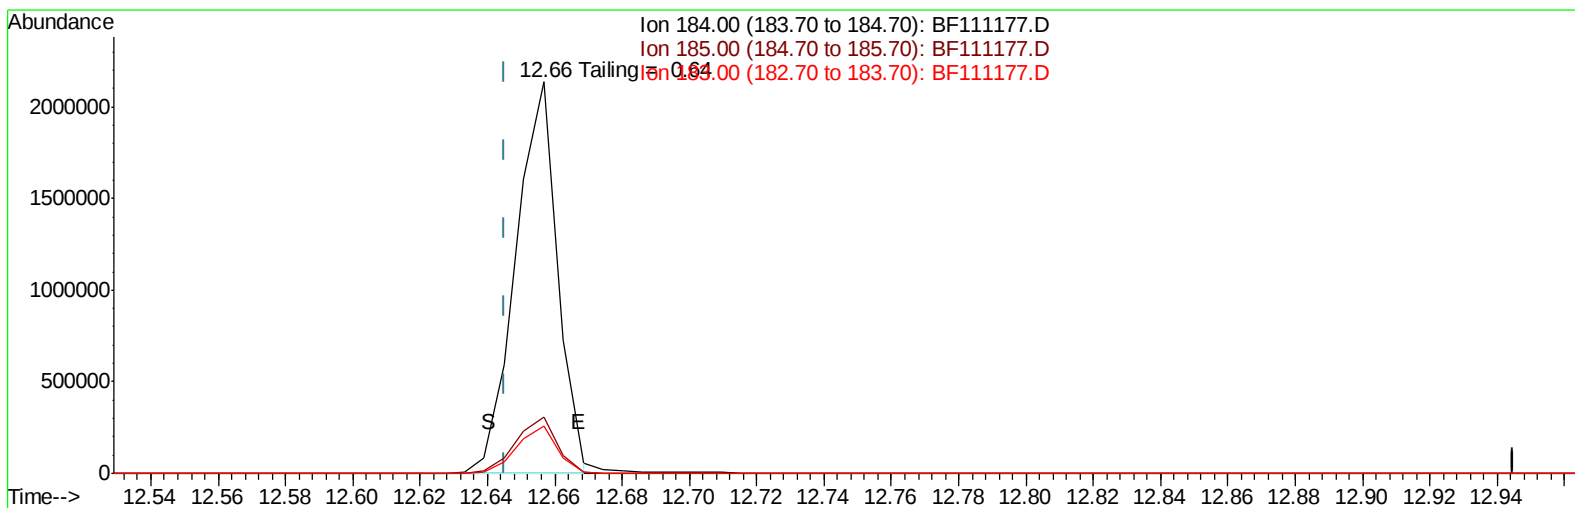

TIC: BF111177.D

(77) Benzidine

12.657min (+0.012) -20.00ng

response 1865312

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.26
183.00	11.10	12.19
0.00	0.00	0.00