
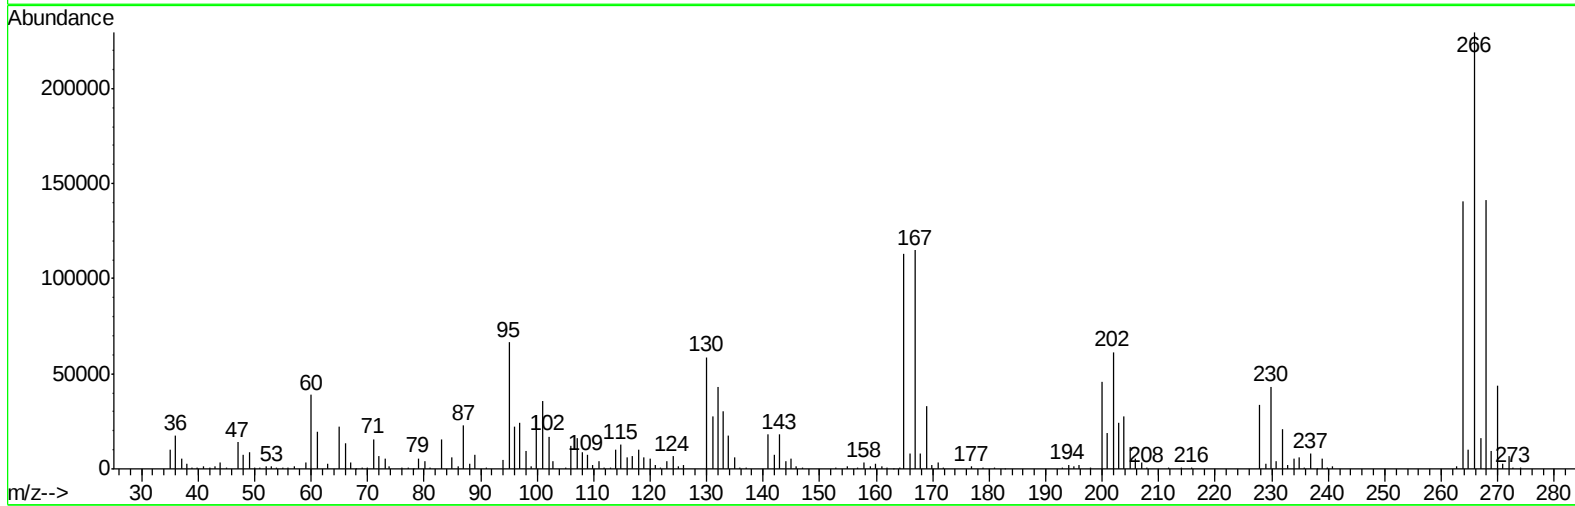


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120718\
Data File : BF111204.D
Acq On : 7 Dec 2018 23:39
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 05:49:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 05 17:30:55 2018
Response via : Initial Calibration

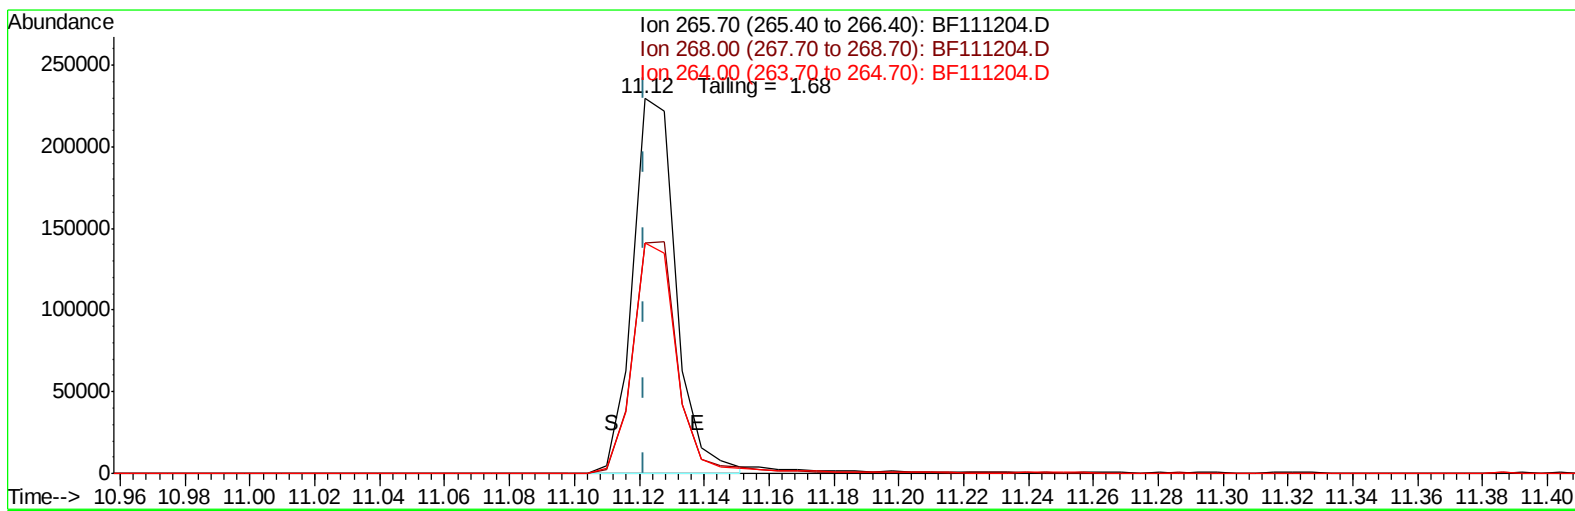

TIC: BF111204.D

(70) Pentachlorophenol (C)



11.122min (+0.000) 11296.68ng

response 222575

Ion	Exp%	Act%
265.70	100	100
268.00	65.30	61.53
264.00	63.50	61.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF120718\
 Data File : BF111204.D
 Acq On : 7 Dec 2018 23:39
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 05:49:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 05 17:30:55 2018
 Response via : Initial Calibration

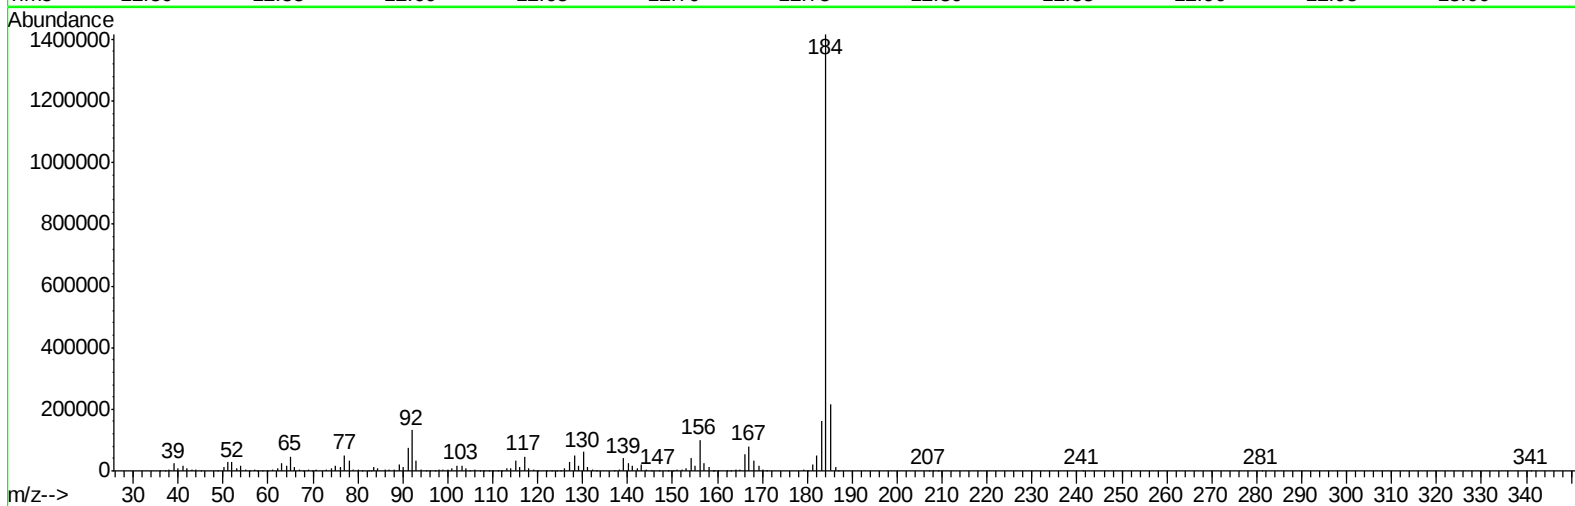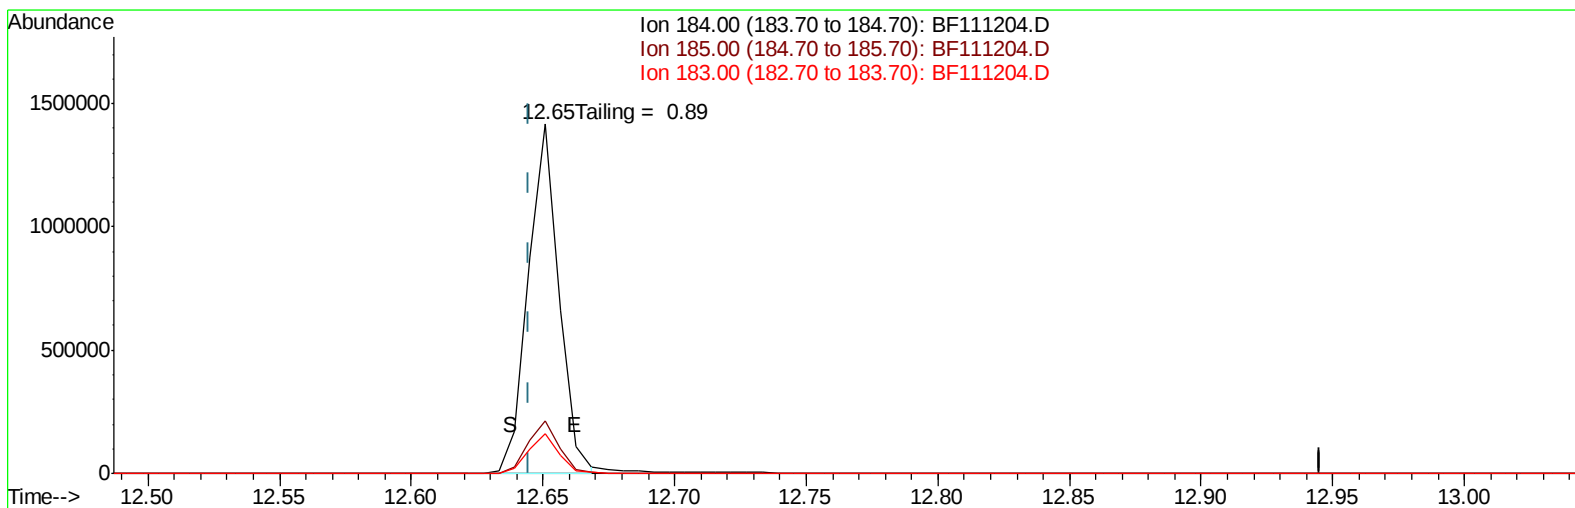

TIC: BF111204.D

(77) Benzidine

12.651min (+0.006) -20.00ng

response 1181371

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	15.16
183.00	11.10	11.34
0.00	0.00	0.00