


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120718\
 Data File : BF111177.D
 Acq On : 7 Dec 2018 10:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 05 17:30:55 2018

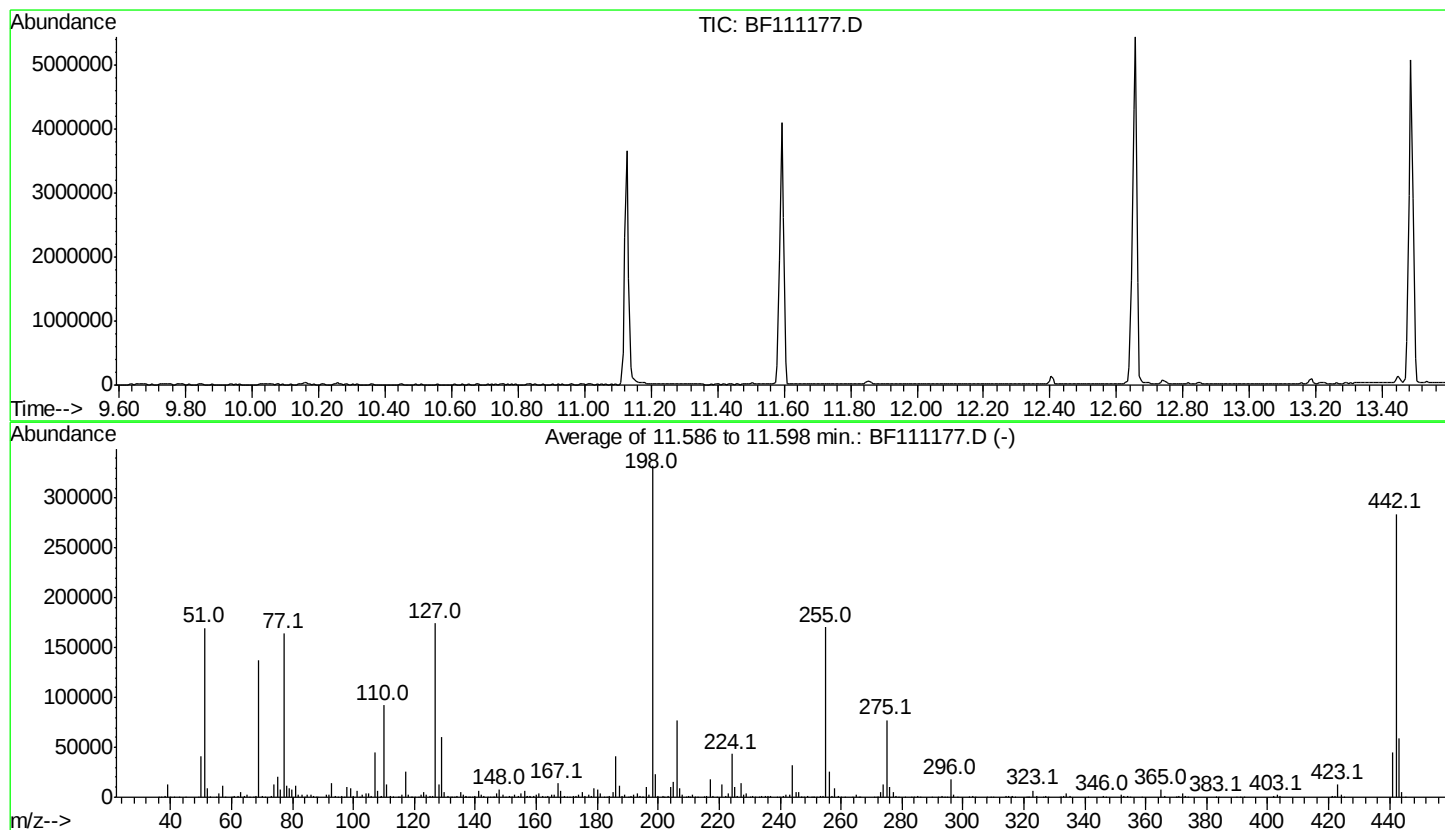

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.0	169586	PASS
68	69	0.00	2	1.4	1897	PASS
69	198	0.00	100	41.4	137606	PASS
70	69	0.00	2	0.7	1013	PASS
127	198	10	80	52.4	174312	PASS
197	198	0.00	2	0.8	2520	PASS
198	198	100	100	100.0	332650	PASS
199	198	5	9	7.0	23296	PASS
275	198	10	60	23.3	77354	PASS
365	198	1	100	2.3	7518	PASS
441	198	0.01	100	13.6	45220	PASS
442	198	50	100	85.4	284186	PASS
443	442	15	24	20.9	59354	PASS