


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120718\
 Data File : BF111204.D
 Acq On : 7 Dec 2018 23:39
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 05 17:30:55 2018

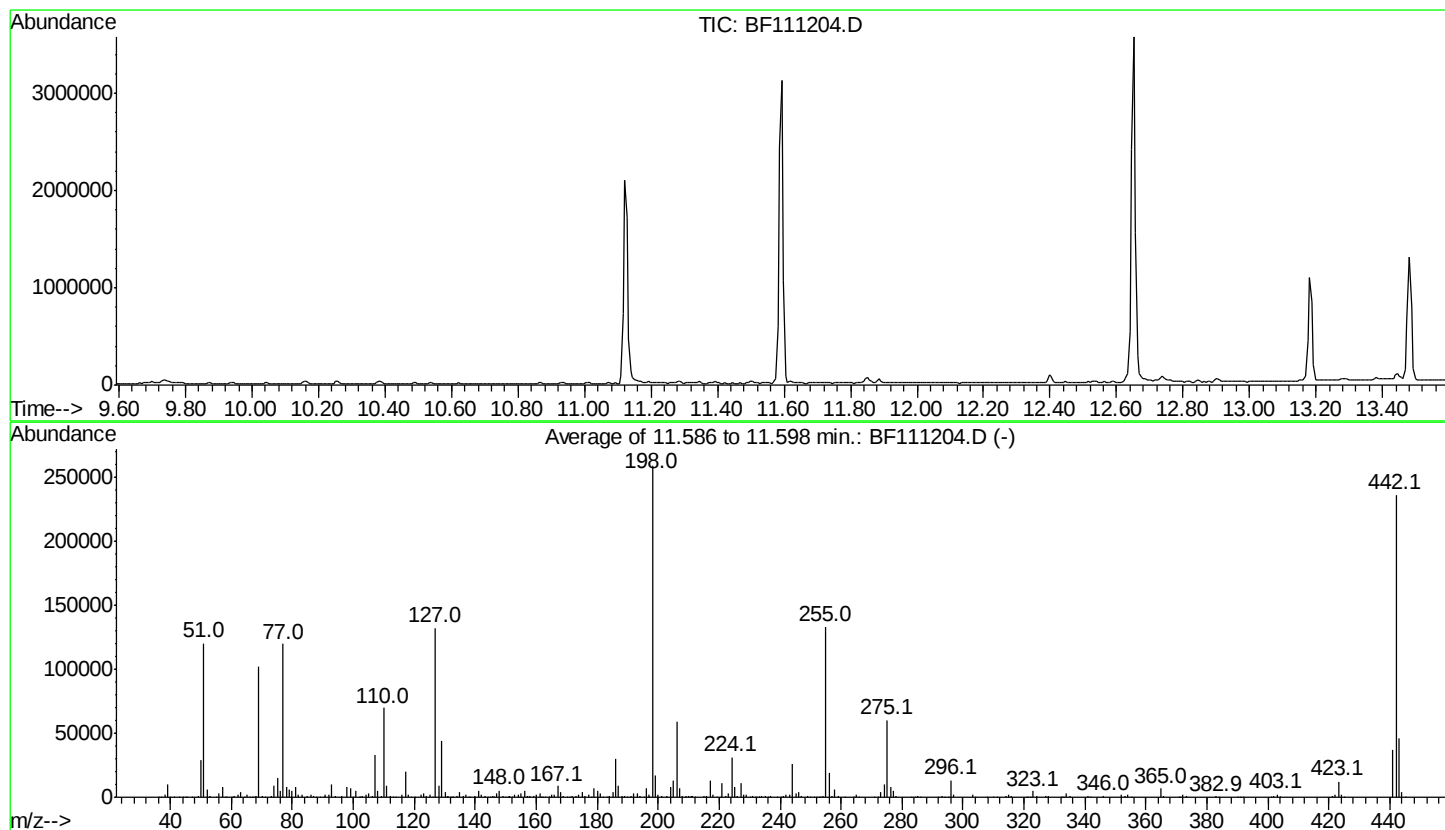

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	120414	PASS
68	69	0.00	2	1.4	1472	PASS
69	198	0.00	100	39.3	101862	PASS
70	69	0.00	2	0.7	718	PASS
127	198	10	80	51.0	132216	PASS
197	198	0.00	2	0.7	1838	PASS
198	198	100	100	100.0	259346	PASS
199	198	5	9	6.6	17024	PASS
275	198	10	60	23.2	60085	PASS
365	198	1	100	2.5	6577	PASS
441	198	0.01	100	14.4	37376	PASS
442	198	50	100	91.2	236480	PASS
443	442	15	24	19.6	46458	PASS