


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF120719\
 Data File : BF118120.D
 Acq On : 7 Dec 2019 10:31
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 06 17:34:43 2019

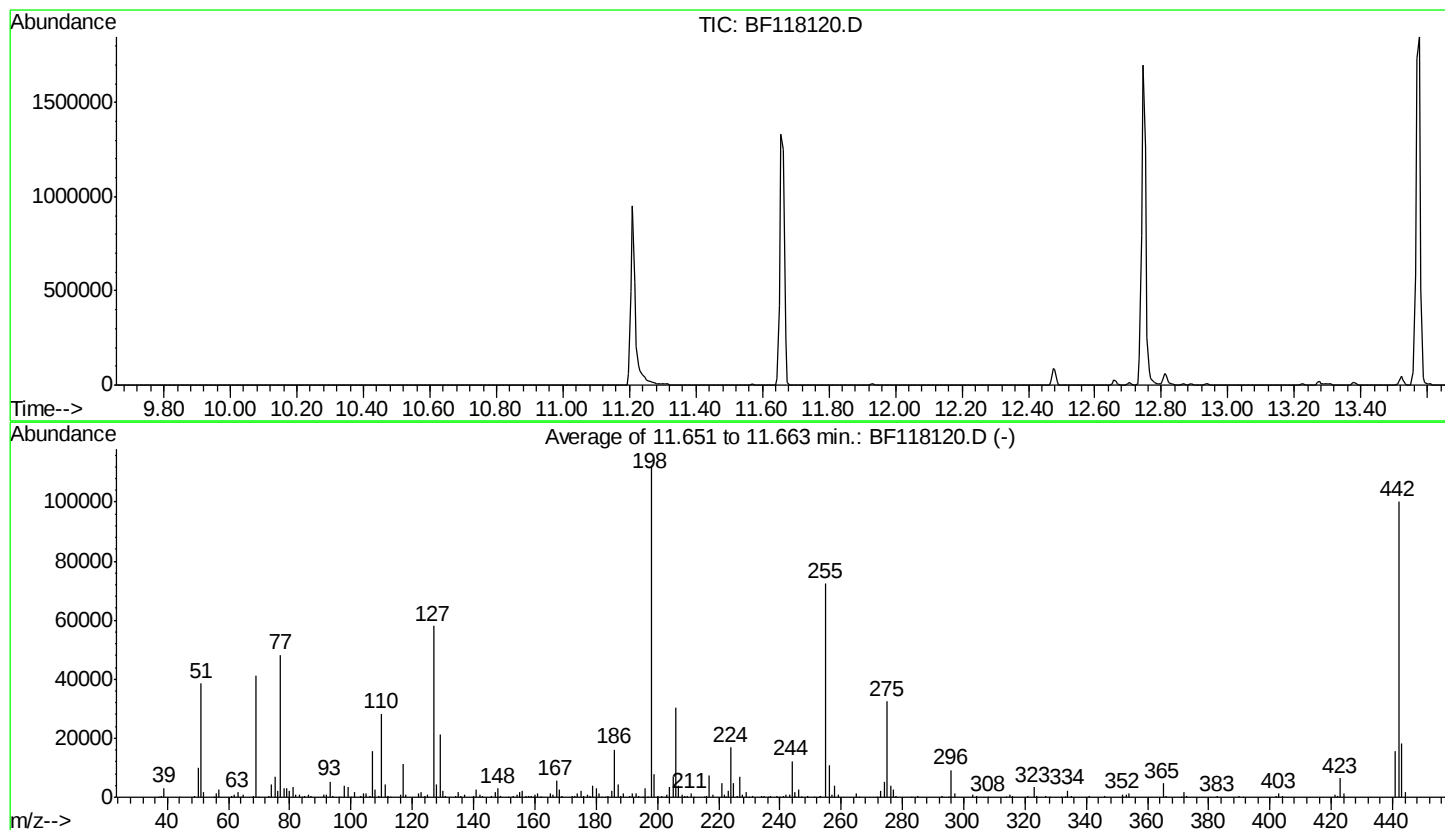

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	38496	PASS
68	69	0.00	2	1.5	622	PASS
69	198	0.00	100	36.6	41104	PASS
70	69	0.00	2	0.4	167	PASS
127	198	10	80	51.6	57949	PASS
197	198	0.00	2	0.2	220	PASS
198	198	100	100	100.0	112357	PASS
199	198	5	9	6.8	7690	PASS
275	198	10	60	28.8	32342	PASS
365	198	1	100	4.1	4573	PASS
441	198	0.01	100	14.0	15680	PASS
442	198	50	100	89.0	100045	PASS
443	442	15	24	18.4	18372	PASS