


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120720\
 Data File : BF122566.D
 Acq On : 7 Dec 2020 10:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 07 12:08:49 2020

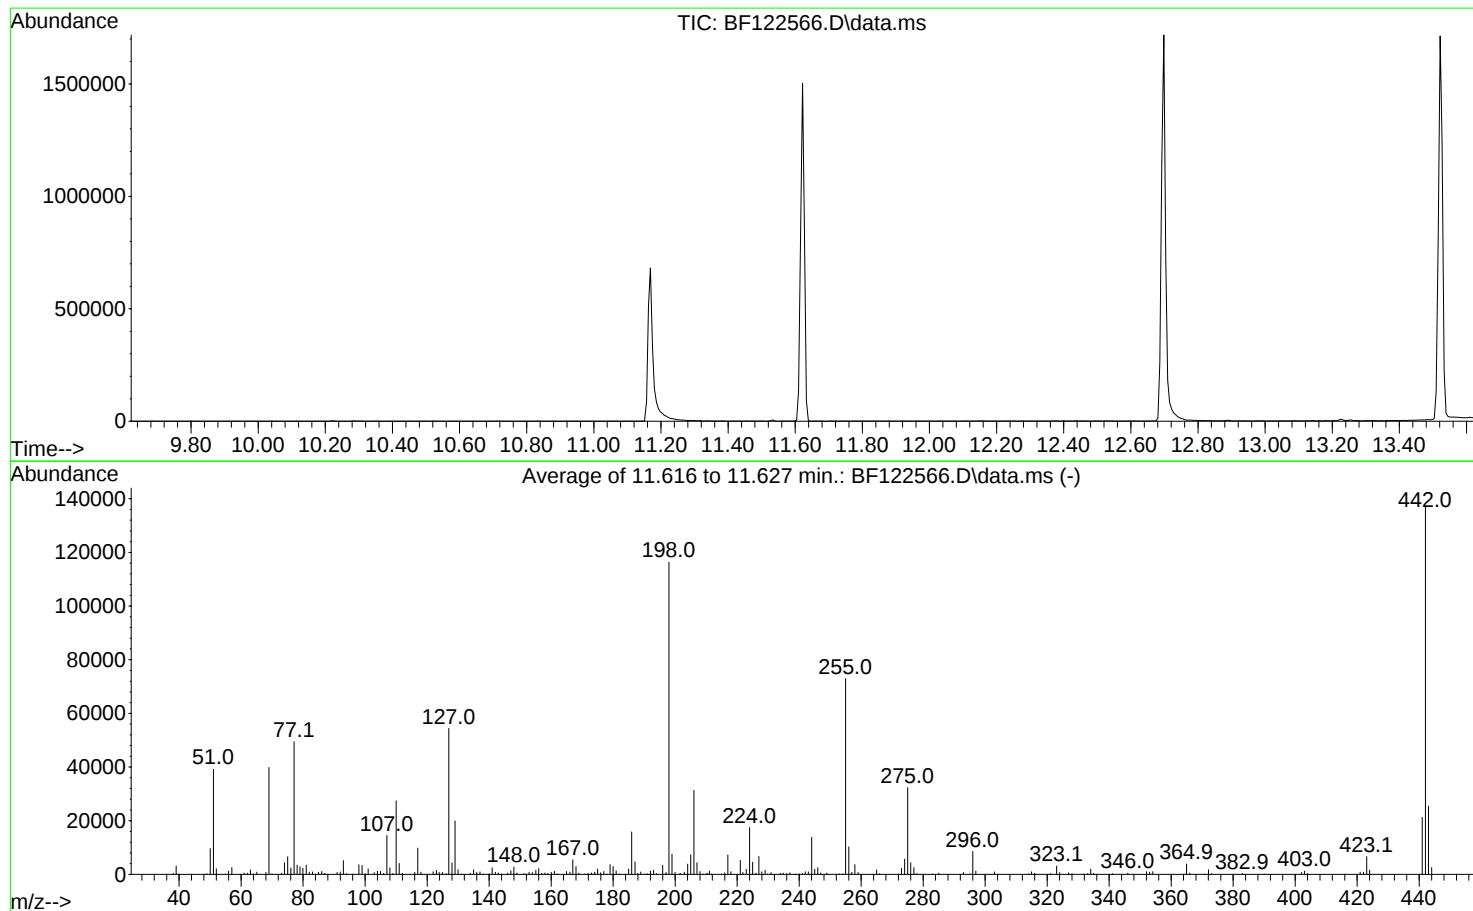

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	39160	PASS
68	69	0.00	2	1.9	775	PASS
69	198	0.00	100	34.2	39832	PASS
70	69	0.00	2	0.5	204	PASS
127	198	10	80	46.7	54368	PASS
197	198	0.00	2	0.6	667	PASS
198	198	100	100	100.0	116360	PASS
199	198	5	9	6.5	7563	PASS
275	198	10	60	27.8	32304	PASS
365	198	1	100	3.3	3869	PASS
441	198	0.01	100	18.3	21253	PASS
442	442	100	100	100.0	137104	PASS
443	442	15	24	18.5	25428	PASS