
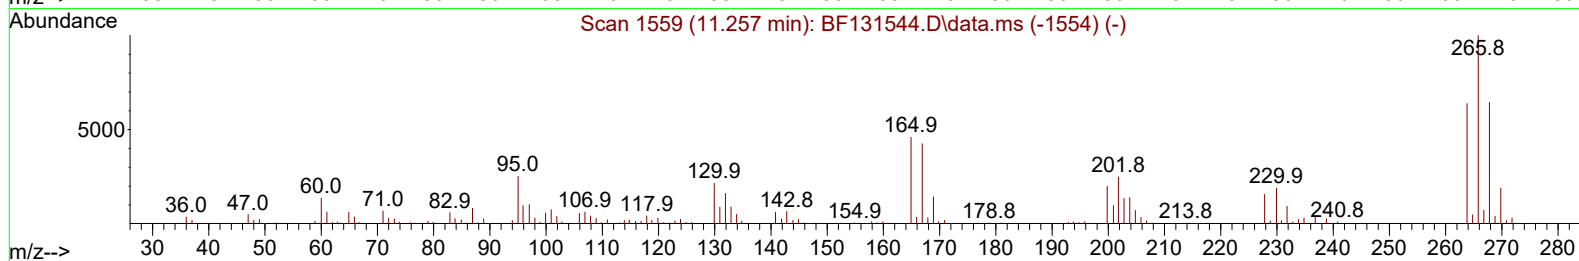
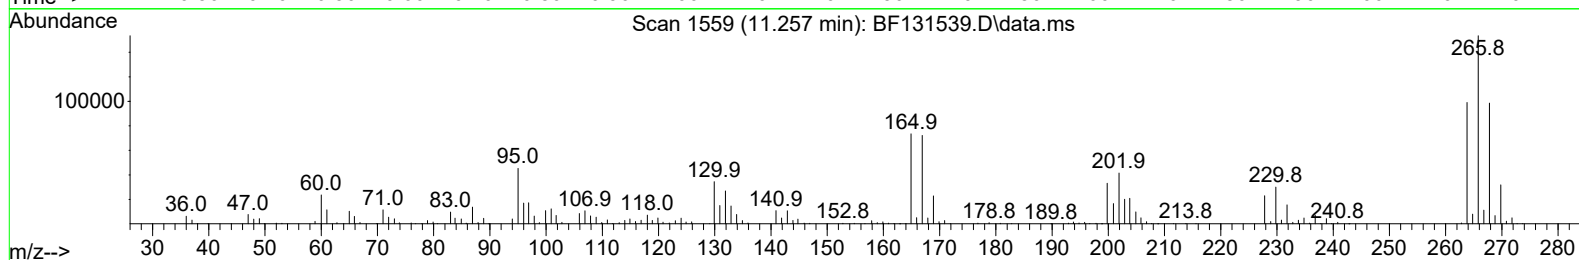


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120722\
 Data File : BF131539.D
 Acq On : 07 Dec 2022 16:16
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 06:28:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 08 04:25:30 2022
 Response via : Initial Calibration

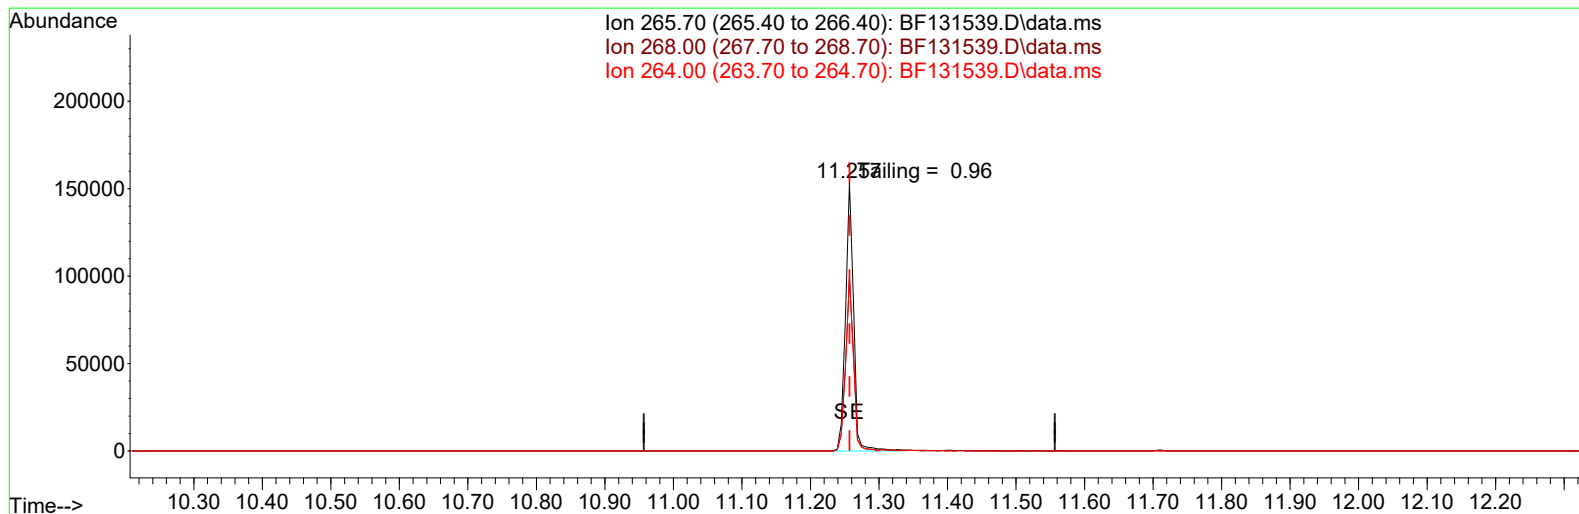

TIC: BF131539.D\data.ms

(70) Pentachlorophenol (C)




11.257min (-0.000) 23001.77 ng

response 124962

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.18
264.00	63.80	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120722\
Data File : BF131539.D
Acq On : 07 Dec 2022 16:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 06:28:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 08 04:25:30 2022
Response via : Initial Calibration

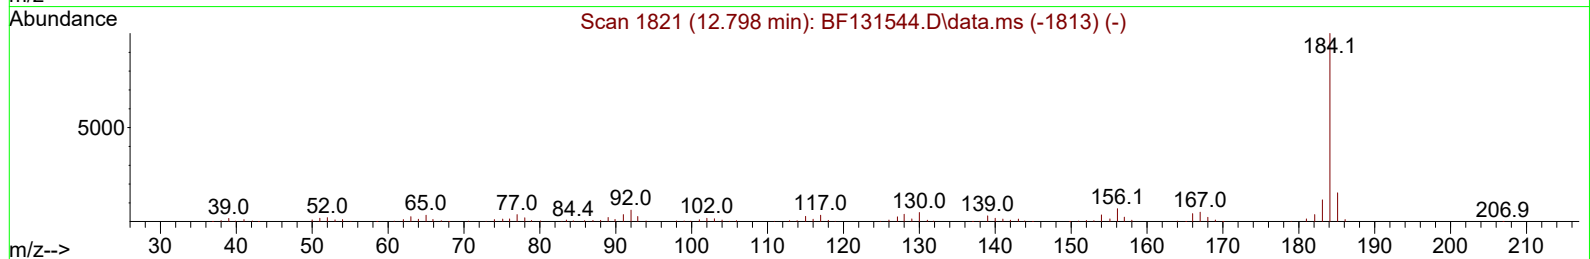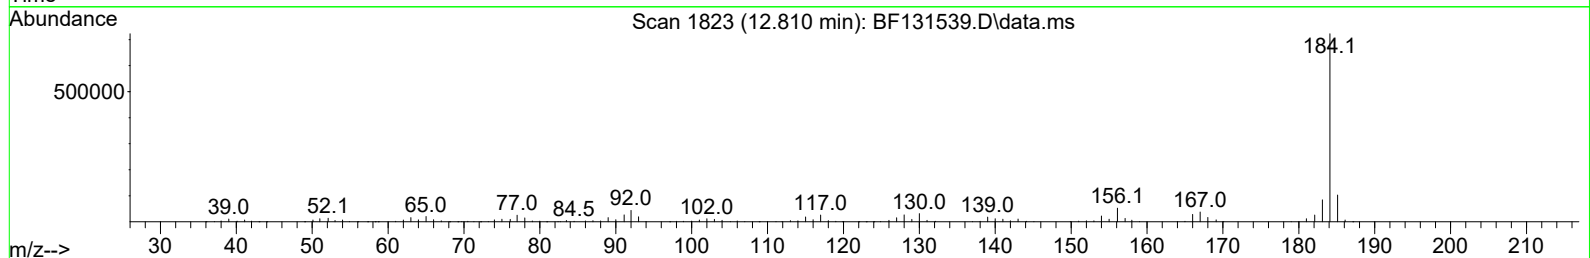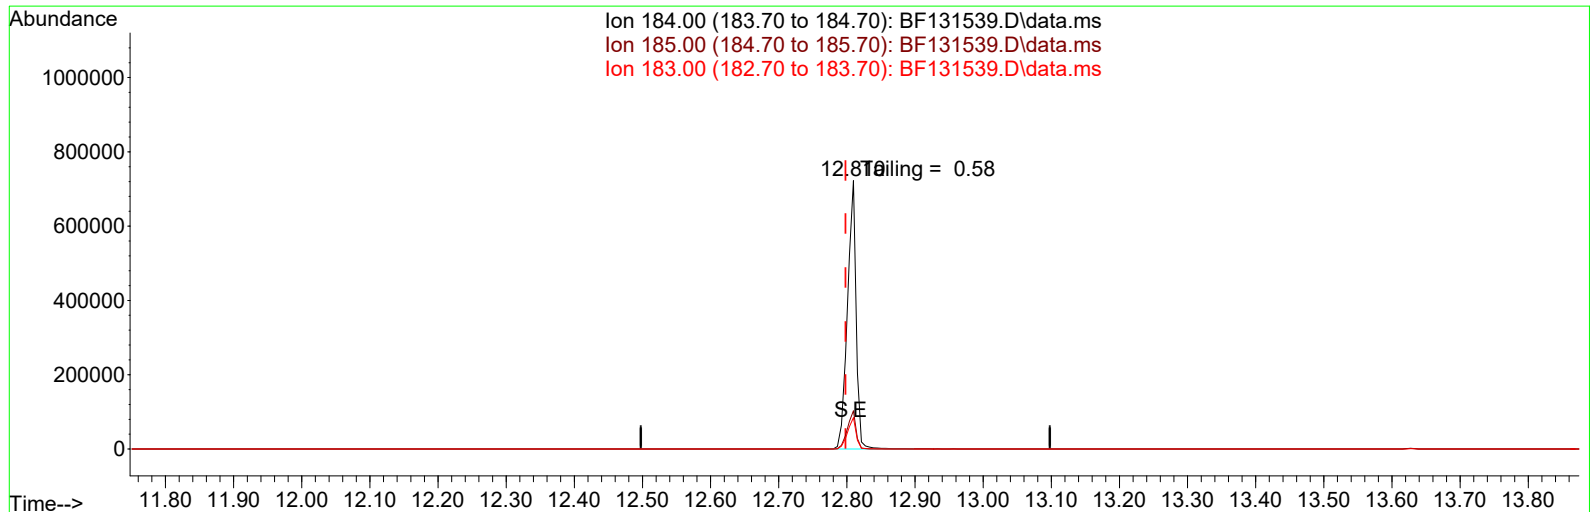

TIC: BF131539.D\data.ms

(77) Benzidine

12.810min (+ 0.012) 0.00 ng

response 639545

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.27
183.00	11.60	11.73
0.00	0.00	0.00