


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120722\
 Data File : BF131539.D
 Acq On : 07 Dec 2022 16:16
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 08 04:25:30 2022

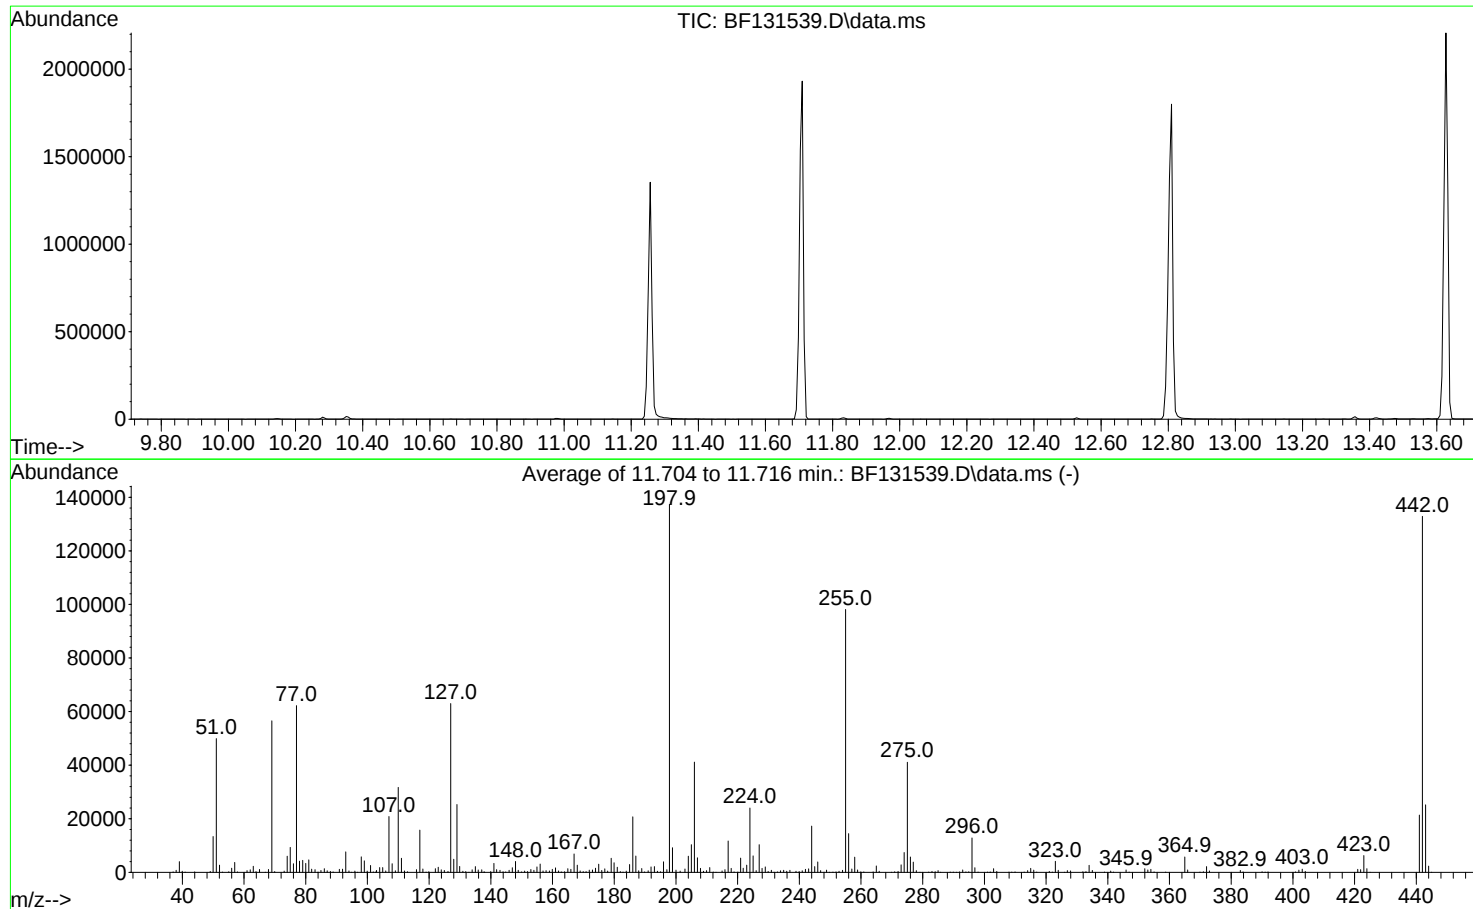




AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	49915	PASS
68	69	0.00	2	1.9	1072	PASS
69	198	0.00	100	41.2	56553	PASS
70	69	0.00	2	0.4	253	PASS
127	198	10	80	45.9	62976	PASS
197	198	0.00	2	0.7	971	PASS
198	198	100	100	100.0	137339	PASS
199	198	5	9	6.7	9147	PASS
275	198	10	60	29.9	41078	PASS
365	198	1	100	4.1	5689	PASS
441	198	0.01	100	15.6	21362	PASS
442	442	50	100	100.0	132869	PASS
443	442	15	24	18.9	25157	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120722\
 Data File : BF131539.D
 Acq On : 07 Dec 2022 16:16
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 08 06:28:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 08 04:25:30 2022
 Response via : Initial Calibration

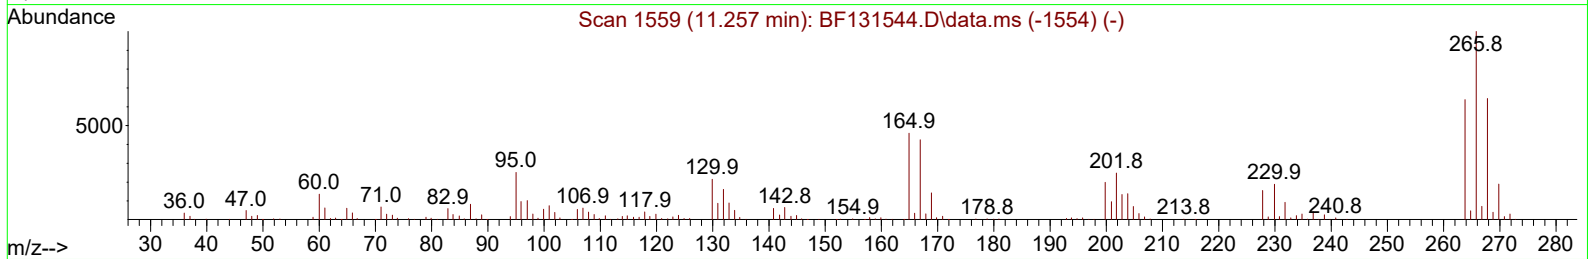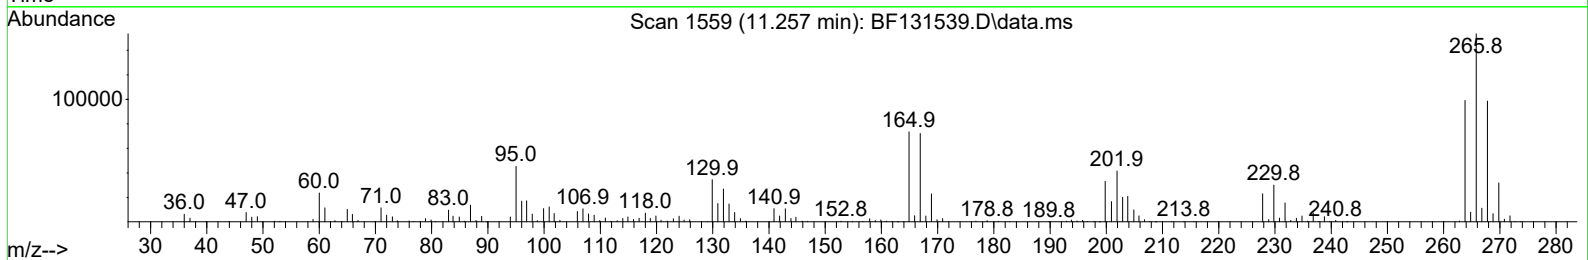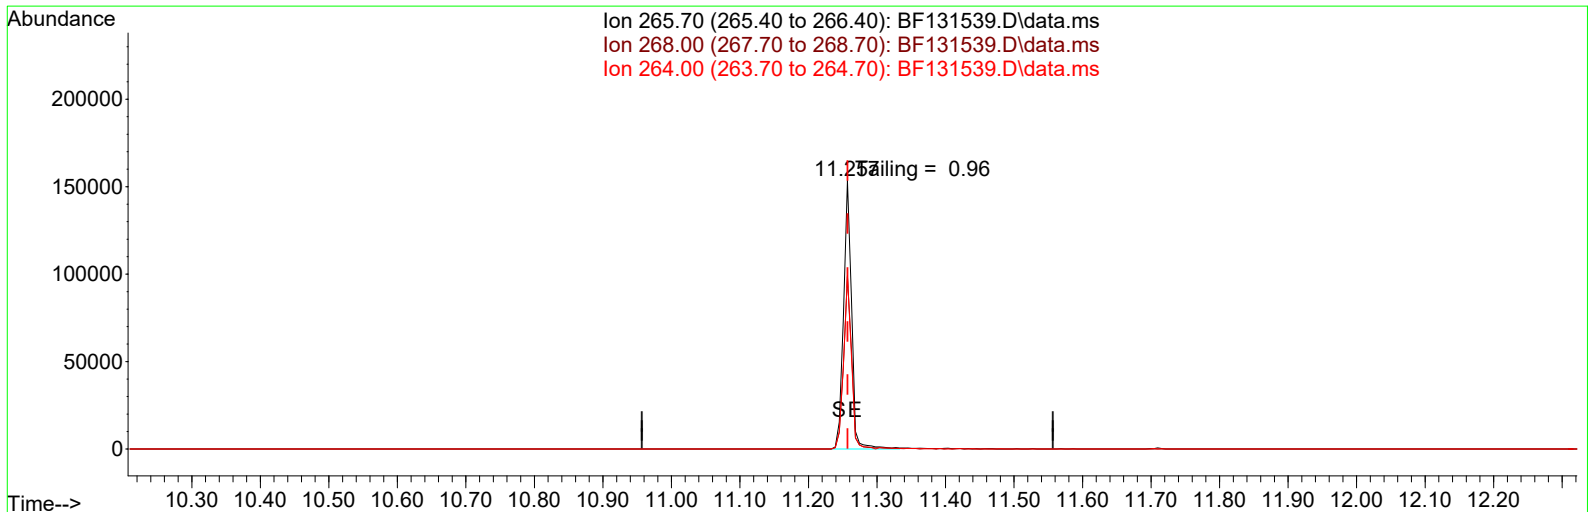

TIC: BF131539.D\data.ms

(70) Pentachlorophenol (C)

11.257min (-0.000) 23001.77 ng




response 124962

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.18
264.00	63.80	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120722\
Data File : BF131539.D
Acq On : 07 Dec 2022 16:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 08 06:28:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 08 04:25:30 2022
Response via : Initial Calibration

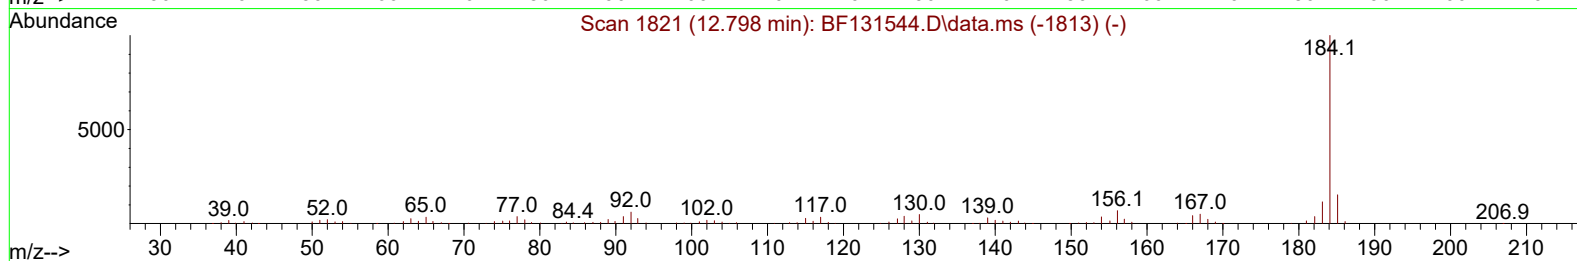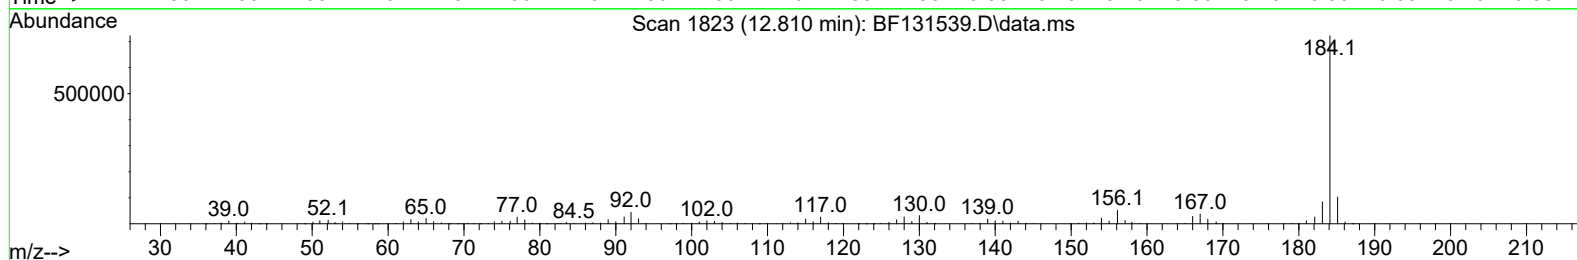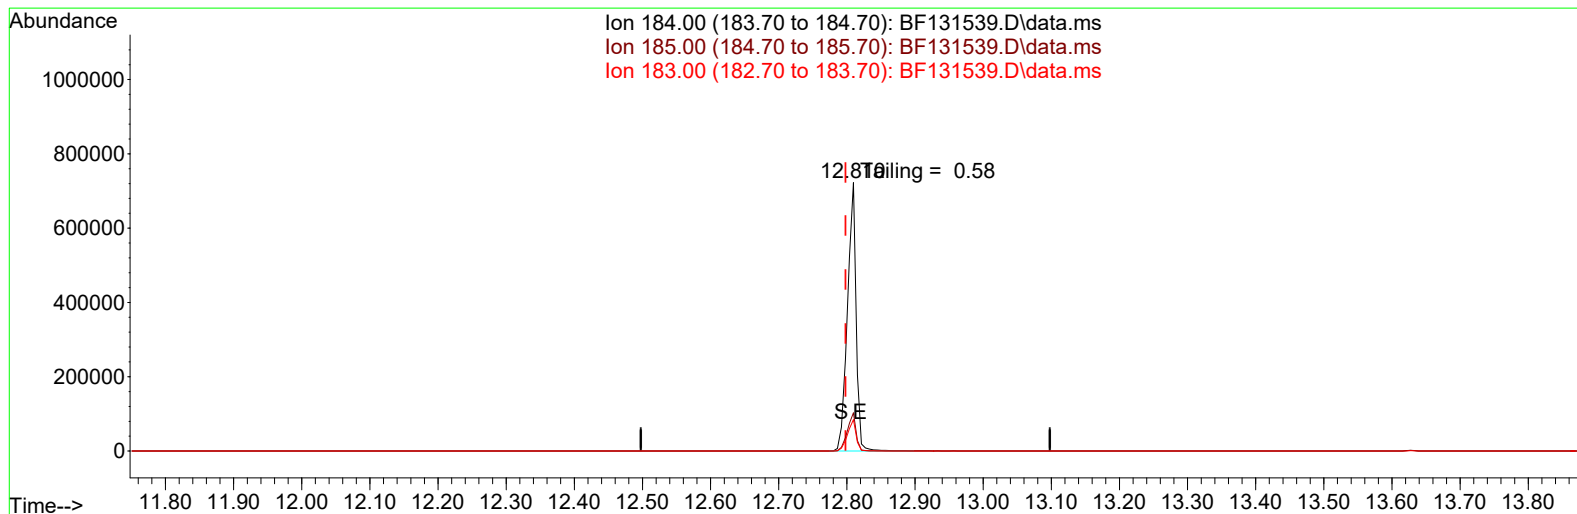

TIC: BF131539.D\data.ms

(77) Benzidine

12.810min (+ 0.012) 0.00 ng

response 639545

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.27
183.00	11.60	11.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/7/2022	BNA_F	<u>BF131539.D</u>
Compound Name	Response	Retention Time
DDT	336666	13.627
DDD	2824	13.357
DDE	0	12.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2824	339490	0.83

Instrument :
BNA_F
ClientSampleId :
DFTPP