

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG120815\  
 Data File : BG020022.D  
 Acq On : 8 Dec 2015 17:40  
 Operator : UM/SJ  
 Sample : G4676-20  
 Misc :  
 ALS Vial : 31 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 MW-12A

Quant Time: Dec 09 04:06:08 2015  
 Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG120215.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 02 18:50:01 2015  
 Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|-----------------------------|-------|------|----------|--------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 8.11  | 152  | 17284    | 20.00  | ng    | -0.03    |
| 21) Naphthalene-d8          | 10.93 | 136  | 76447    | 20.00  | ng    | -0.02    |
| 38) Acenaphthene-d10        | 14.74 | 164  | 53671    | 20.00  | ng    | -0.03    |
| 63) Phenanthrene-d10        | 17.48 | 188  | 130702   | 20.00  | ng    | -0.03    |
| 75) Chrysene-d12            | 21.75 | 240  | 161737   | 20.00  | ng    | -0.04    |
| 86) Perylene-d12            | 25.03 | 264  | 150185   | 20.00  | ng    | -0.06    |
| System Monitoring Compounds |       |      |          |        |       |          |
| 5) 2-Fluorophenol           | 5.66  | 112  | 63006    | 65.88  | ng    | 0.00     |
| 7) Phenol-d6                | 7.26  | 99   | 56458    | 39.10  | ng    | -0.02    |
| 23) Nitrobenzene-d5         | 9.28  | 82   | 152799   | 102.01 | ng    | -0.02    |
| 41) 2,4,6-Tribromophenol    | 16.22 | 330  | 120011   | 146.14 | ng    | -0.02    |
| 44) 2-Fluorobiphenyl        | 13.37 | 172  | 384609   | 97.85  | ng    | -0.02    |
| 78) Terphenyl-d14           | 20.08 | 244  | 647465   | 97.64  | ng    | -0.03    |


| Target Compounds | Qvalue |
|------------------|--------|
|------------------|--------|


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG120815\  
Data File : BG020022.D  
Acq On : 8 Dec 2015 17:40  
Operator : UM/SJ  
Sample : G4676-20  
Misc :  
ALS Vial : 31 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
MW-12A

Quant Time: Dec 09 04:06:08 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG120215.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 02 18:50:01 2015  
Response via : Initial Calibration

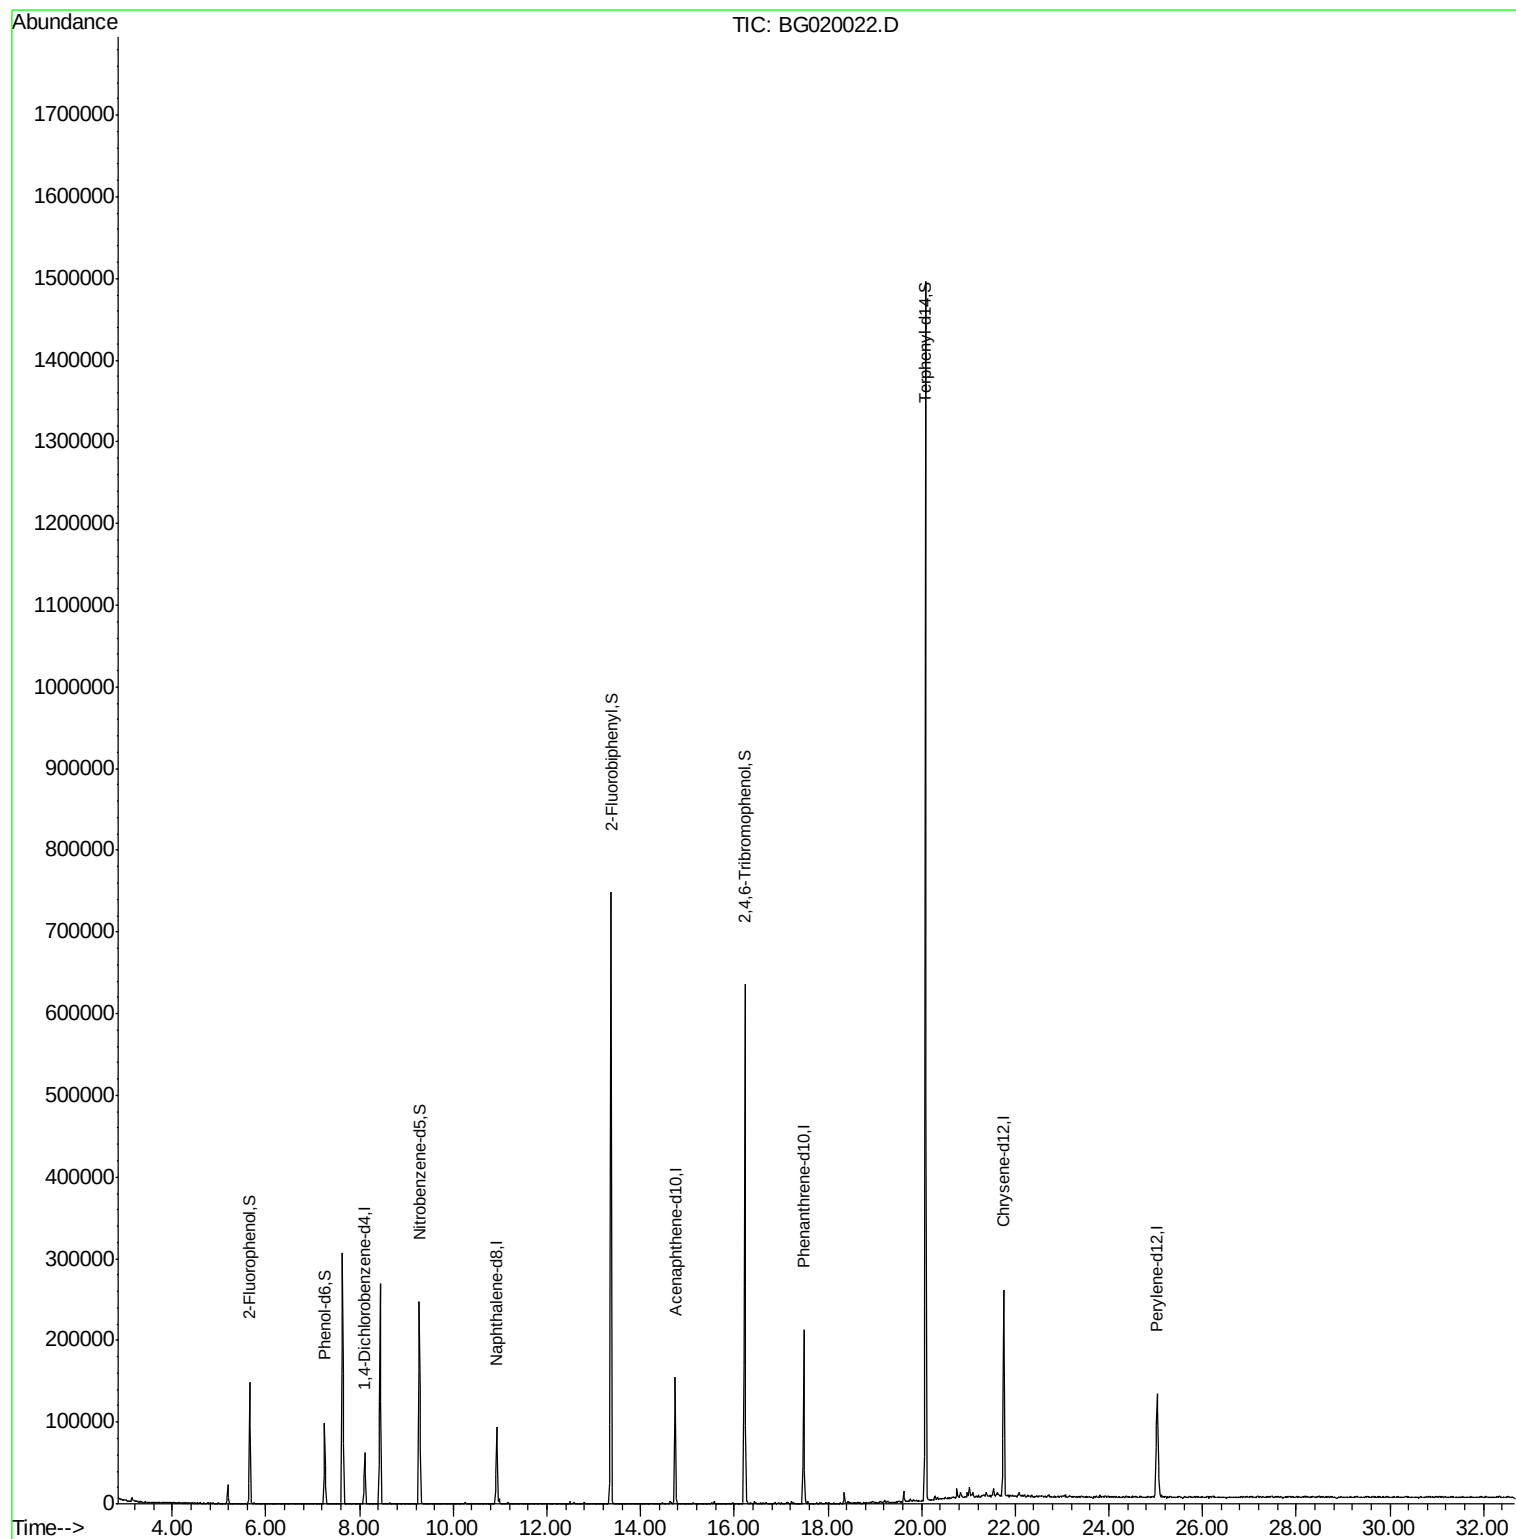




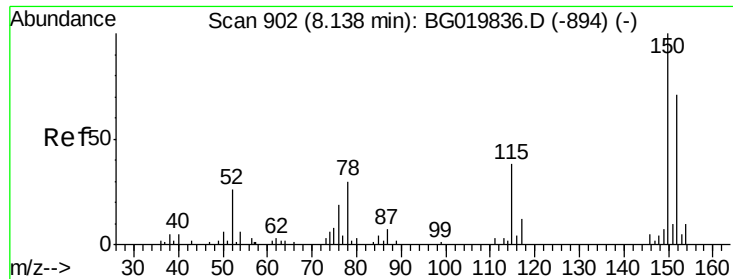


#1

1,4-Dichlorobenzene-d4  
Concen: 20.00 ng  
RT: 8.11 min Scan# 897  
Delta R.T. -0.03 min  
Lab File: BG020022.D  
Acq: 8 Dec 2015 17:40

Instrument :  
BNA\_F  
ClientSampleId :  
MW-12A




Tgt Ion:152 Resp: 17284  
Ion Ratio Lower Upper  
152 100  
150 160.7 115.0 172.4  
115 59.0 43.9 65.9

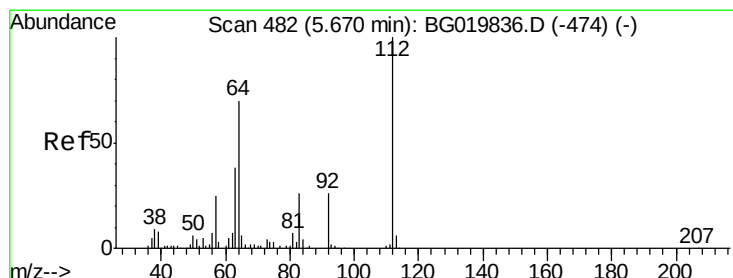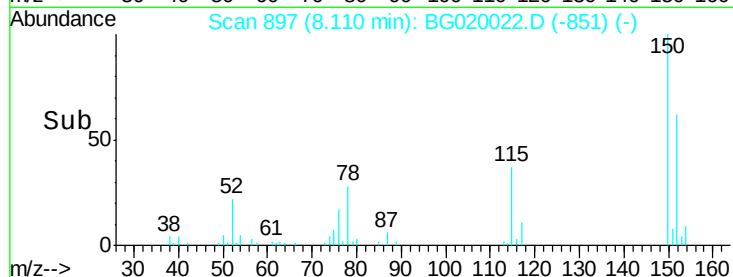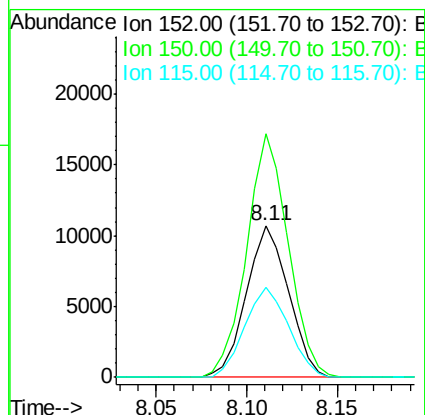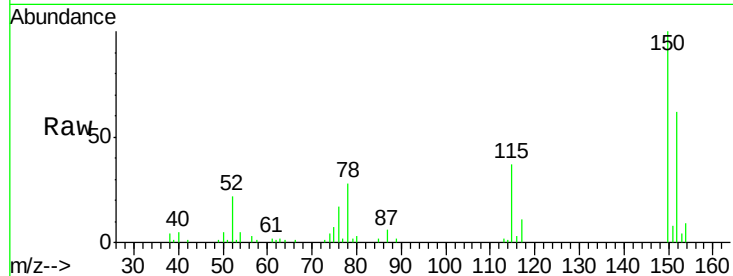


#5

2-Fluorophenol  
Concen: 65.88 ng  
RT: 5.66 min Scan# 480  
Delta R.T. -0.01 min  
Lab File: BG020022.D  
Acq: 8 Dec 2015 17:40

Tgt Ion:112 Resp: 63006  
Ion Ratio Lower Upper  
112 100  
64 62.4 43.7 65.5  
63 35.6 24.0 36.0

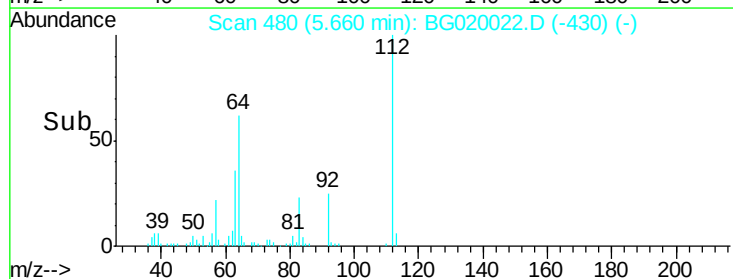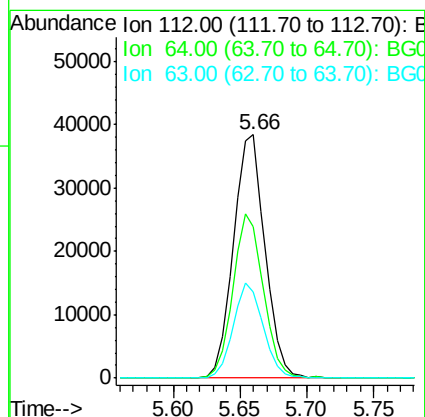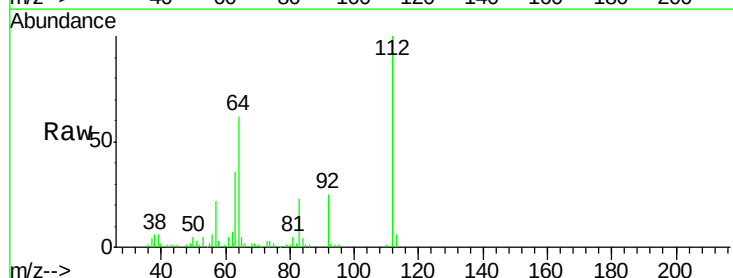

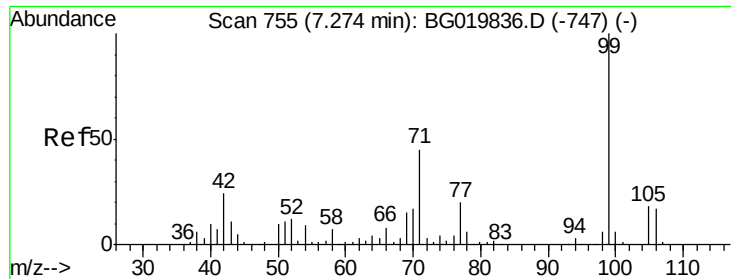

#7

Phenol-d6

Concen: 39.10 ng

RT: 7.26 min Scan# 752

Delta R.T. -0.02 min

Lab File: BG020022.D

Acq: 8 Dec 2015 17:40

Instrument :

BNA\_F

ClientSampleId :

MW-12A


Tgt Ion: 99 Resp: 56458

Ion Ratio Lower Upper




99 100

42 19.1 11.5 17.3#

71 38.1 22.6 34.0#

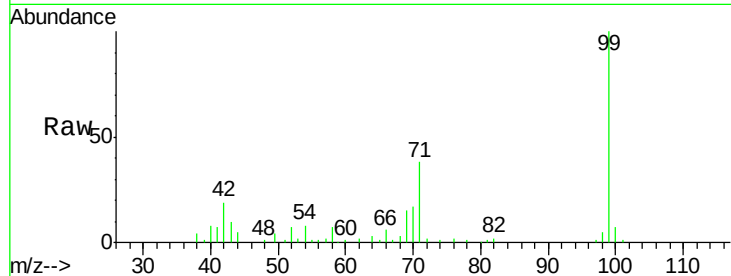

Abundance Ion 99.00 (98.70 to 99.70): BGC  
Ion 42.00 (41.70 to 42.70): BGC  
Ion 71.00 (70.70 to 71.70): BGC

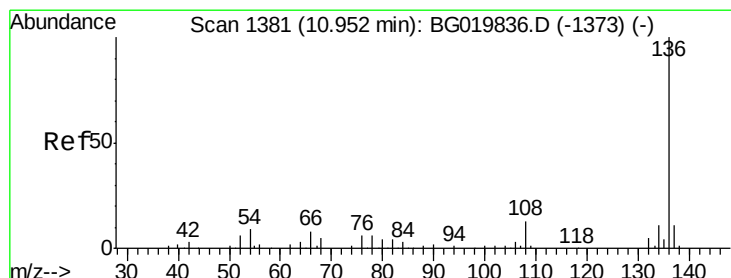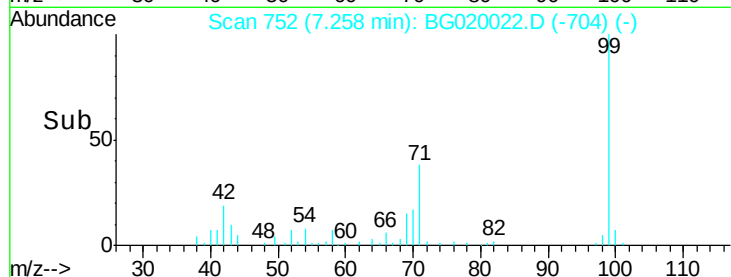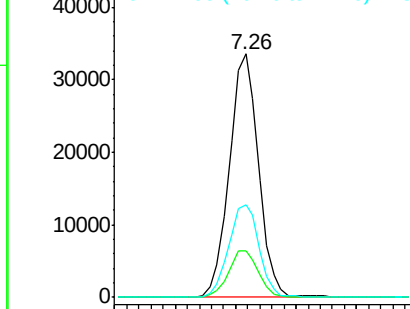

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.93 min Scan# 1377

Delta R.T. -0.02 min

Lab File: BG020022.D

Acq: 8 Dec 2015 17:40

Tgt Ion: 136 Resp: 76447


Ion Ratio Lower Upper

136 100



137 10.4 8.6 12.8


54 8.2 5.4 8.2#

68 5.1 5.3 7.9#

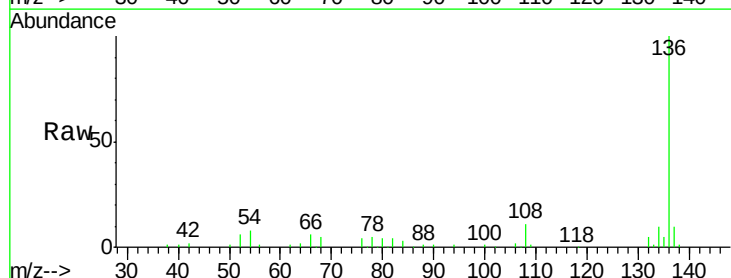

Abundance Ion 136.00 (135.70 to 136.70): BGC  
Ion 137.00 (136.70 to 137.70): BGC  
Ion 54.00 (53.70 to 54.70): BGC  
Ion 68.00 (67.70 to 68.70): BGC



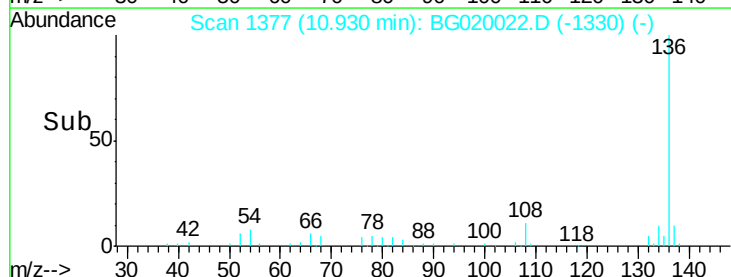
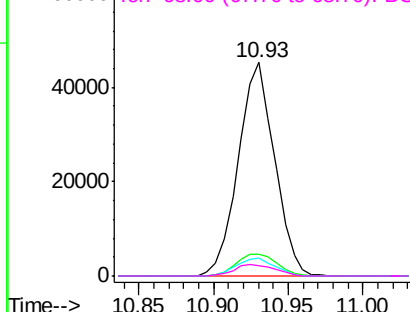


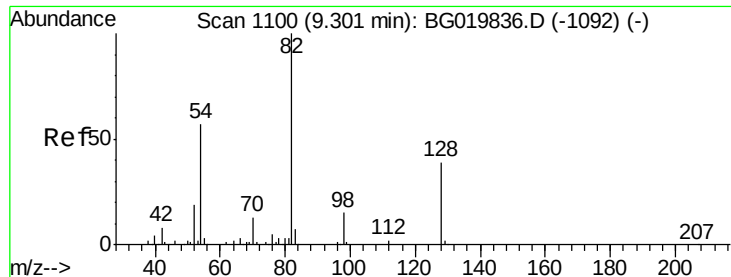

#23  
 Nitrobenzene-d5  
 Concen: 102.01 ng  
 RT: 9.28 min Scan# 1096  
 Delta R.T. -0.02 min  
 Lab File: BG020022.D  
 Acq: 8 Dec 2015 17:40




Instrument :  
 BNA\_F  
 ClientSampleId :  
 MW-12A


Tgt Ion: 82 Resp: 152799  
 Ion Ratio Lower Upper  
 82 100  
 128 39.6 36.7 55.1  
 54 49.5 33.8 50.8

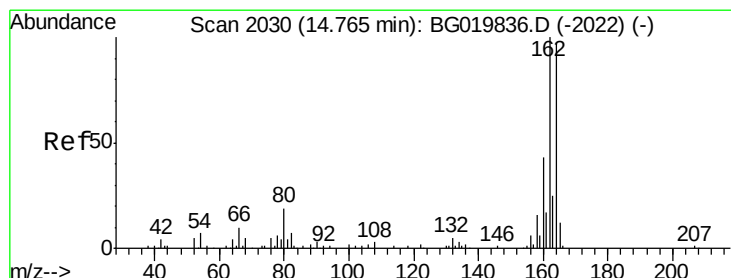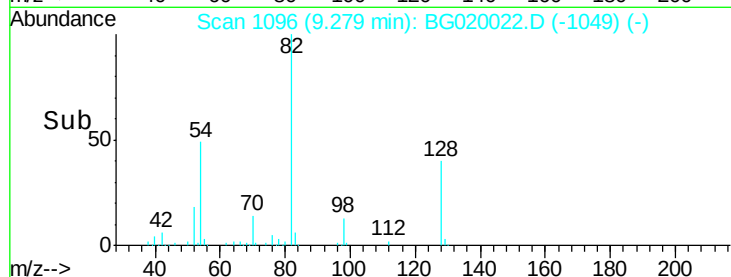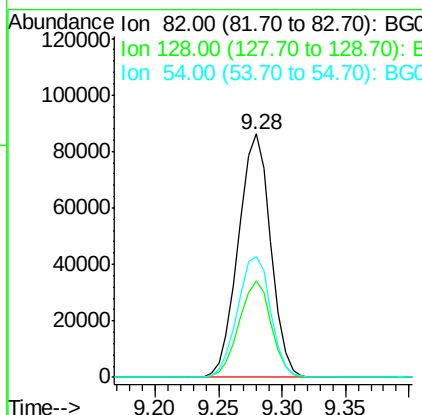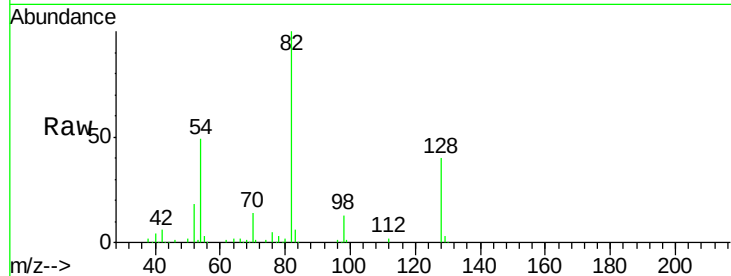

#38  
 Acenaphthene-d10  
 Concen: 20.00 ng  
 RT: 14.74 min Scan# 2025  
 Delta R.T. -0.03 min  
 Lab File: BG020022.D  
 Acq: 8 Dec 2015 17:40

Tgt Ion: 164 Resp: 53671  
 Ion Ratio Lower Upper  
 164 100  
 162 104.6 78.8 118.2  
 160 44.8 36.4 54.6

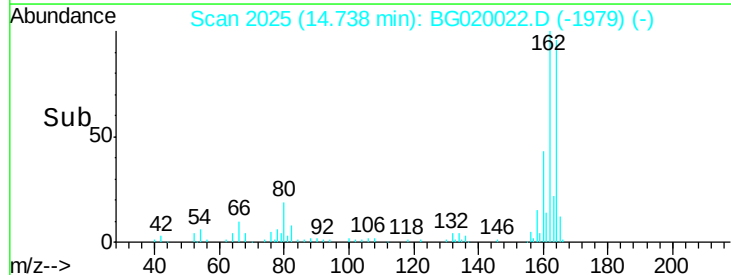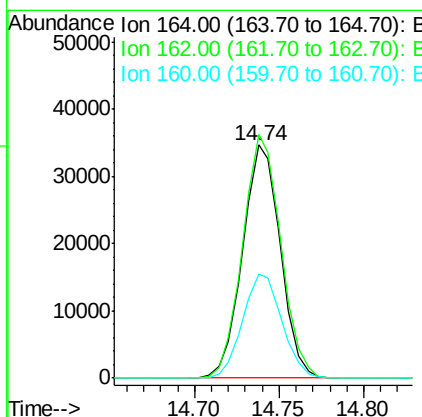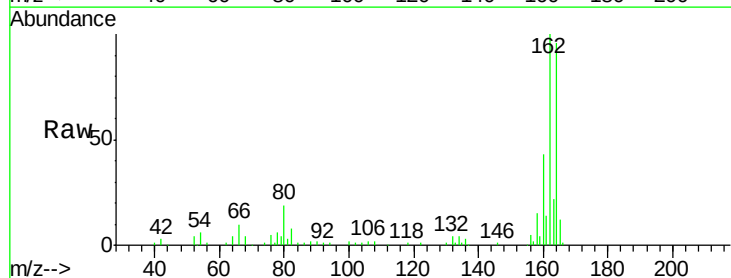


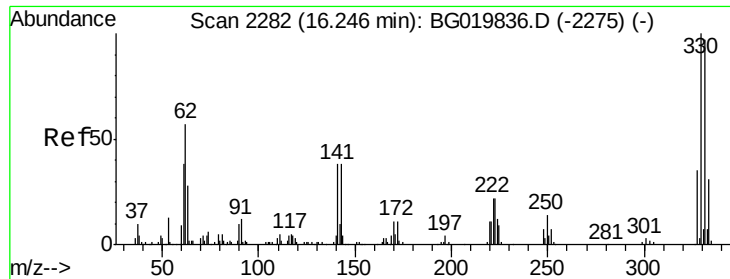




#41  
 2,4,6-Tribromophenol  
 Concen: 146.14 ng  
 RT: 16.22 min Scan# 2278  
 Delta R.T. -0.02 min  
 Lab File: BG020022.D  
 Acq: 8 Dec 2015 17:40

Instrument :  
 BNA\_F  
 ClientSampleId :  
 MW-12A

Tgt Ion:330 Resp: 120011  
 Ion Ratio Lower Upper  
 330 100  
 332 96.0 78.1 117.1  
 141 37.0 28.2 42.2

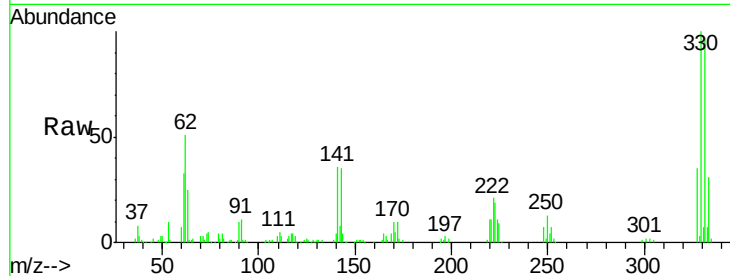


Abundance Ion 329.80 (329.50 to 330.50): E  
 Ion 331.80 (331.50 to 332.50): E  
 Ion 141.00 (140.70 to 141.70): E

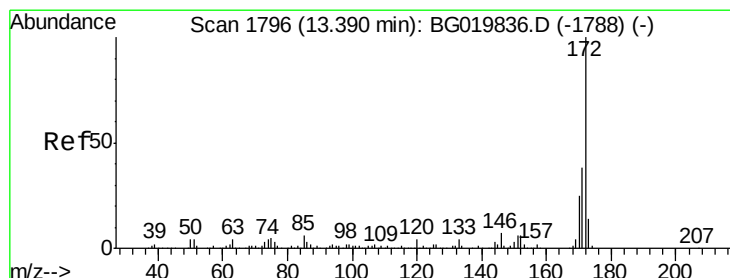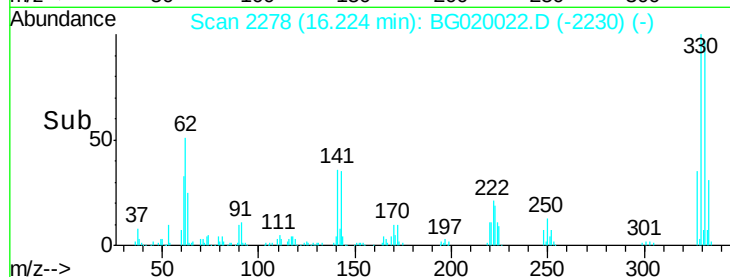
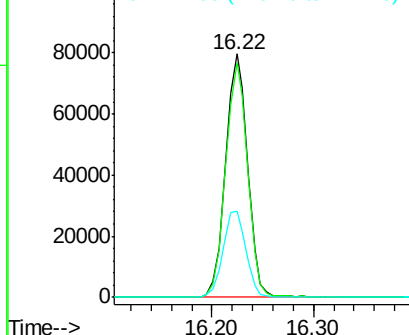



#44  
 2-Fluorobiphenyl  
 Concen: 97.85 ng  
 RT: 13.37 min Scan# 1792  
 Delta R.T. -0.02 min  
 Lab File: BG020022.D  
 Acq: 8 Dec 2015 17:40

Tgt Ion:172 Resp: 384609  
 Ion Ratio Lower Upper  
 172 100  
 171 37.3 29.0 43.6  
 170 24.7 19.9 29.9

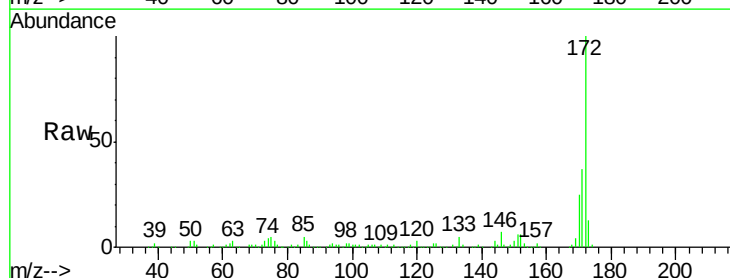

Abundance Ion 172.00 (171.70 to 172.70): E  
 Ion 171.00 (170.70 to 171.70): E  
 Ion 170.00 (169.70 to 170.70): E



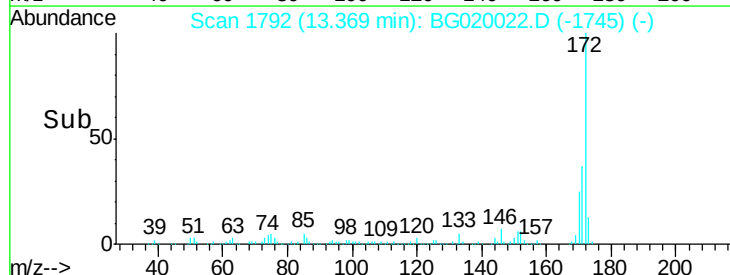
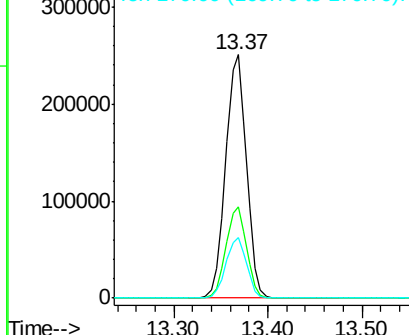


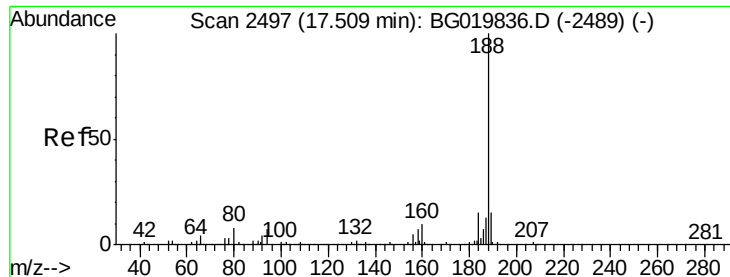

#63  
Phenanthrene-d10  
Concen: 20.00 ng  
RT: 17.48 min Scan# 2492  
Delta R.T. -0.03 min  
Lab File: BG020022.D  
Acq: 8 Dec 2015 17:40




Instrument :  
BNA\_F  
ClientSampleId :  
MW-12A


Tgt Ion:188 Resp: 130702  
Ion Ratio Lower Upper  
188 100  
94 7.5 7.7 11.5#  
80 8.9 7.8 11.8

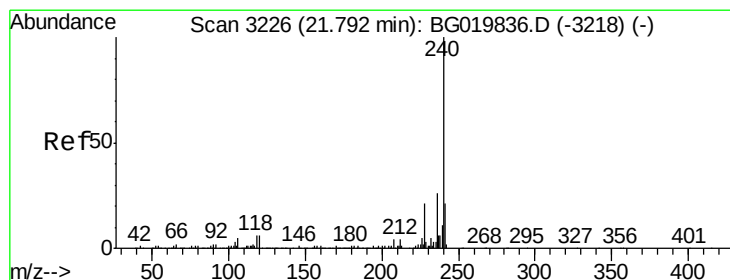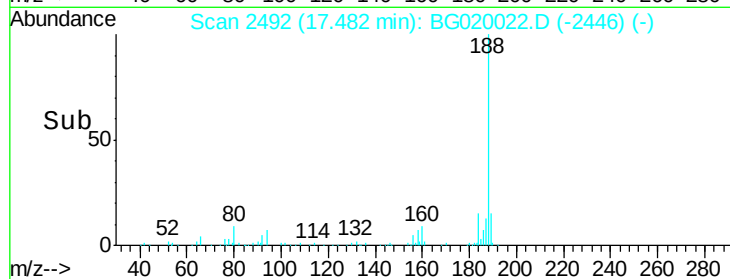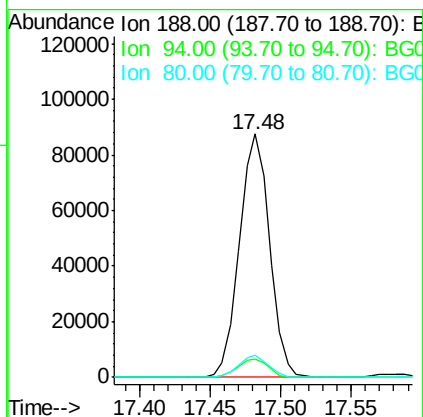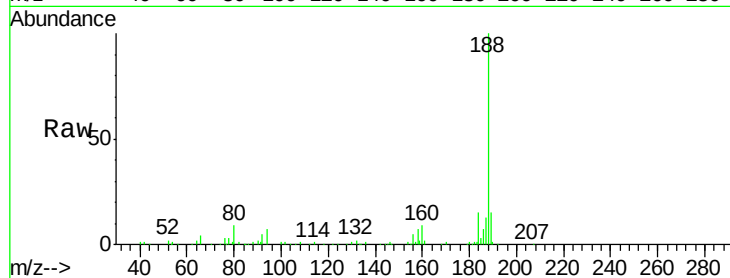

#75  
Chrysene-d12  
Concen: 20.00 ng  
RT: 21.75 min Scan# 3219  
Delta R.T. -0.04 min  
Lab File: BG020022.D  
Acq: 8 Dec 2015 17:40

Tgt Ion:240 Resp: 161737  
Ion Ratio Lower Upper  
240 100  
120 6.9 7.4 11.0#  
236 24.8 20.7 31.1

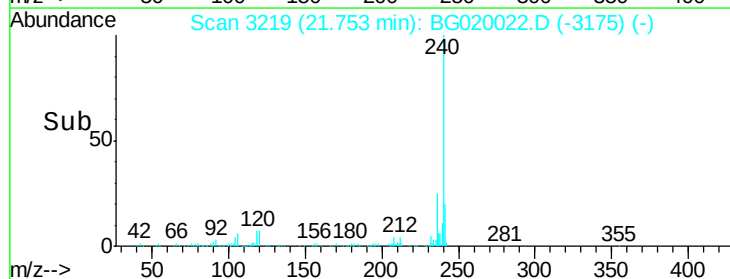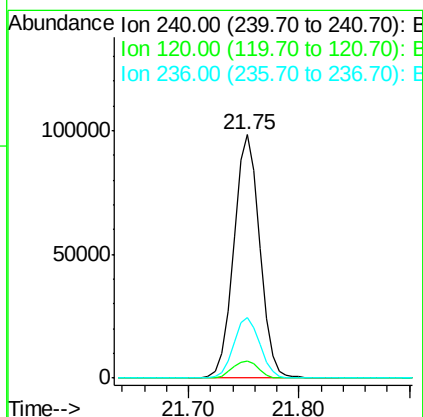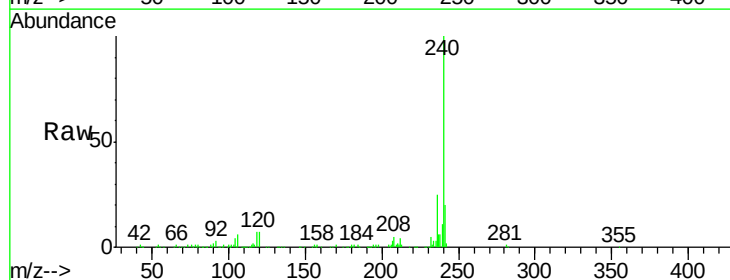

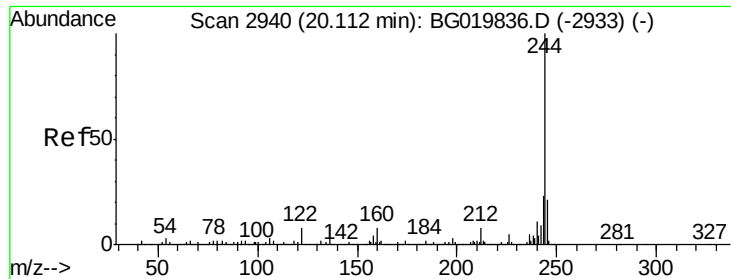

#78

Terphenyl-d14

Concen: 97.64 ng

RT: 20.08 min Scan# 2935

Delta R.T. -0.03 min

Lab File: BG020022.D

Acq: 8 Dec 2015 17:40

Instrument :

BNA\_F

ClientSampleId :

MW-12A


Tgt Ion:244 Resp: 647465

Ion Ratio Lower Upper

244 100

212 8.3 6.9 10.3




122 8.0 10.2 15.2#

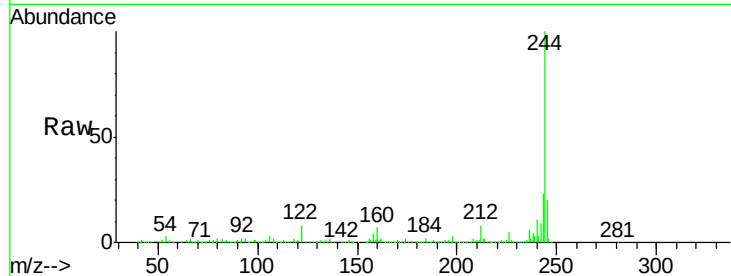

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

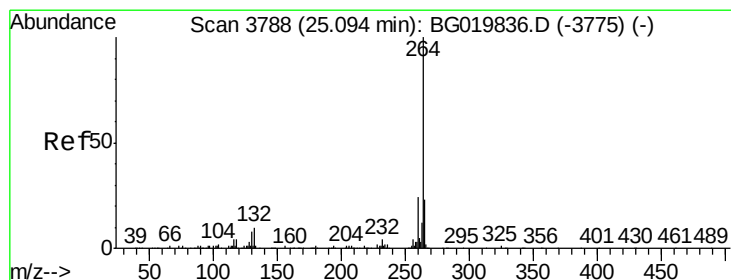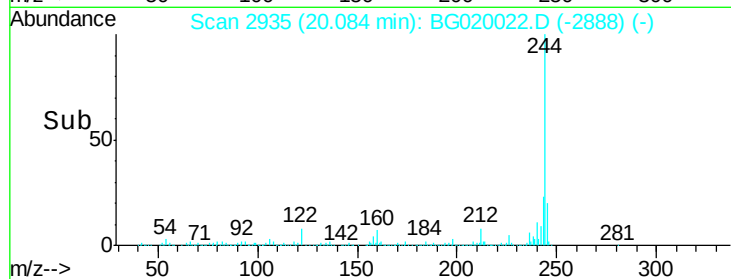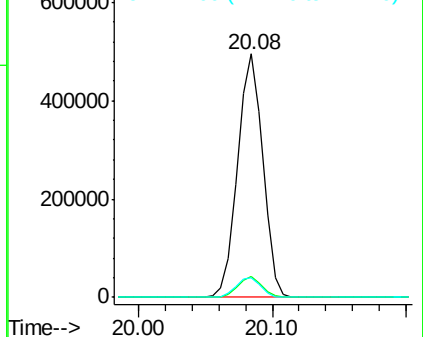

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.03 min Scan# 3777

Delta R.T. -0.06 min

Lab File: BG020022.D

Acq: 8 Dec 2015 17:40


Tgt Ion:264 Resp: 150185

Ion Ratio Lower Upper

264 100

260 24.6 18.5 27.7

265 22.2 17.2 25.8

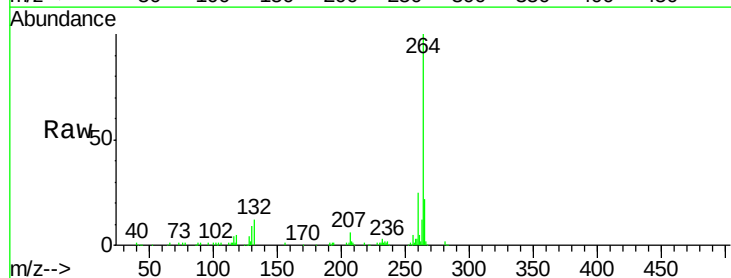

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

