



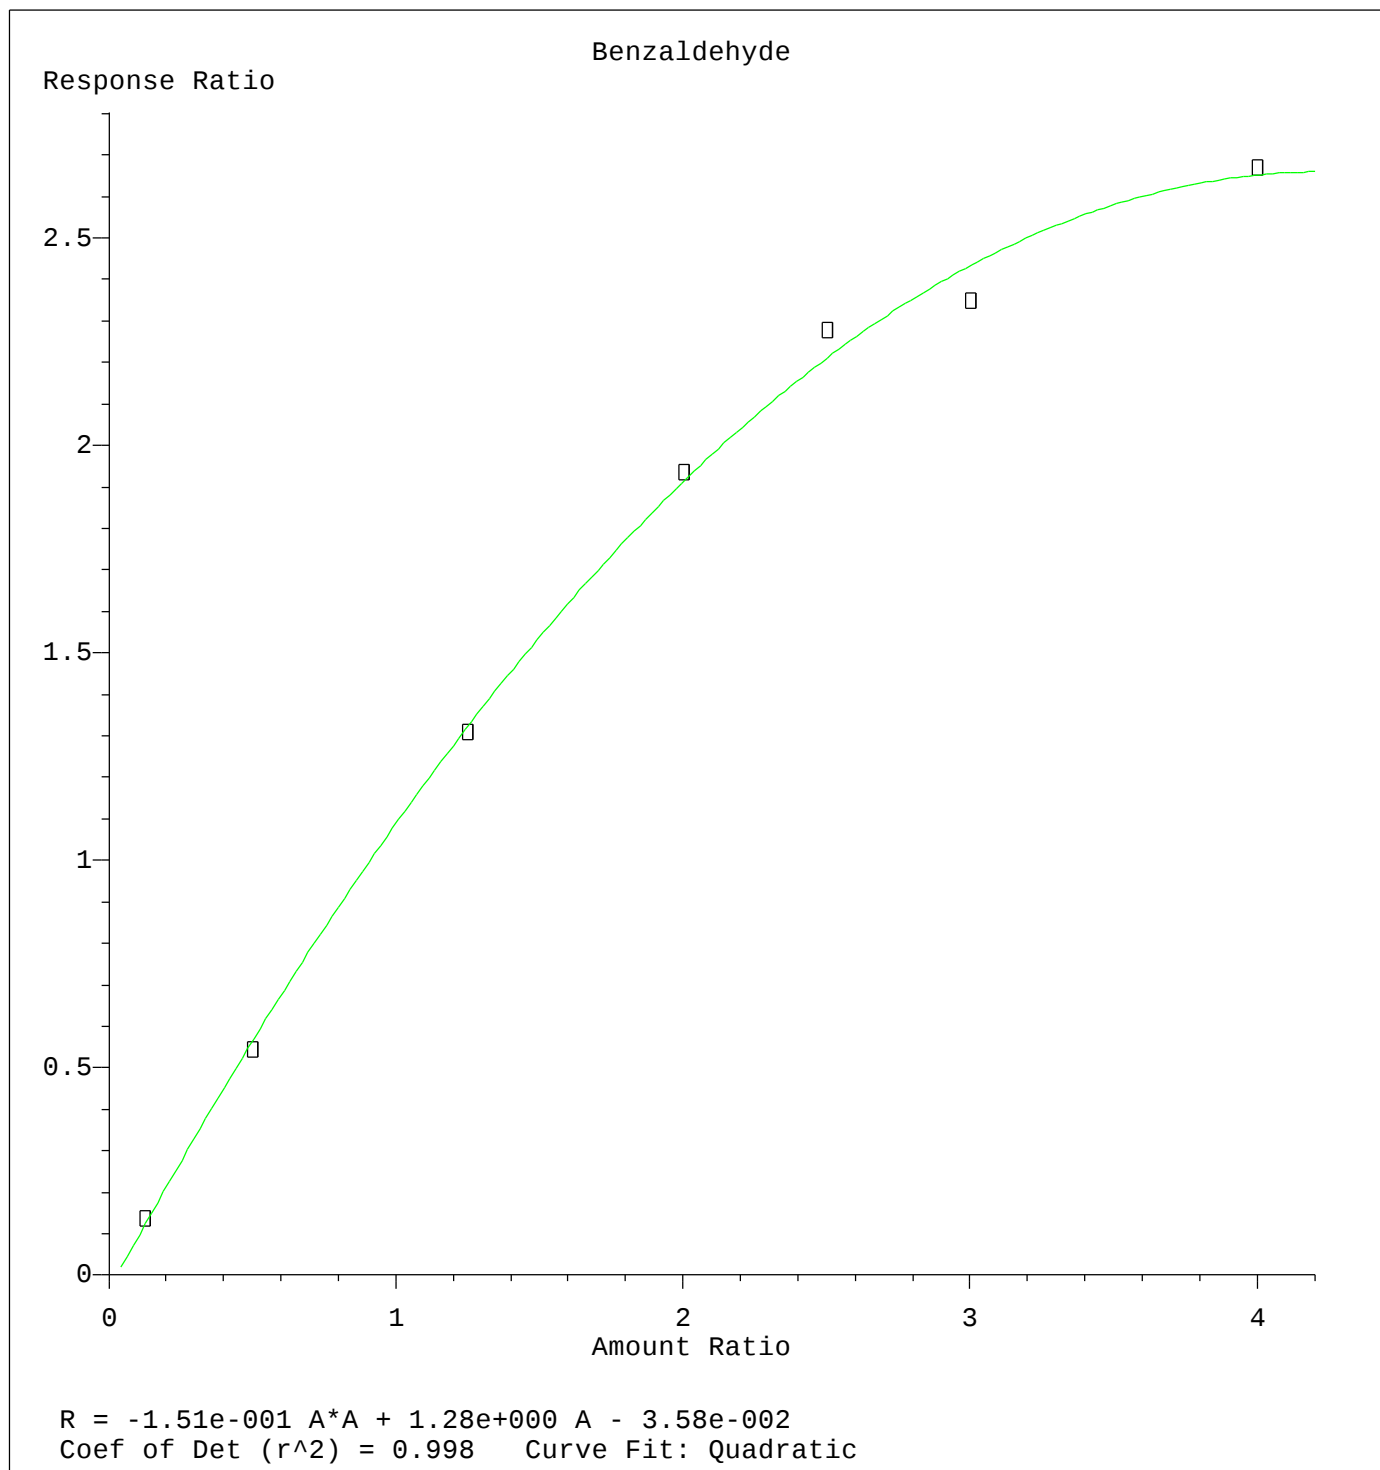


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Calibration Table Last Updated: Wed Dec 09 00:23:35 2015

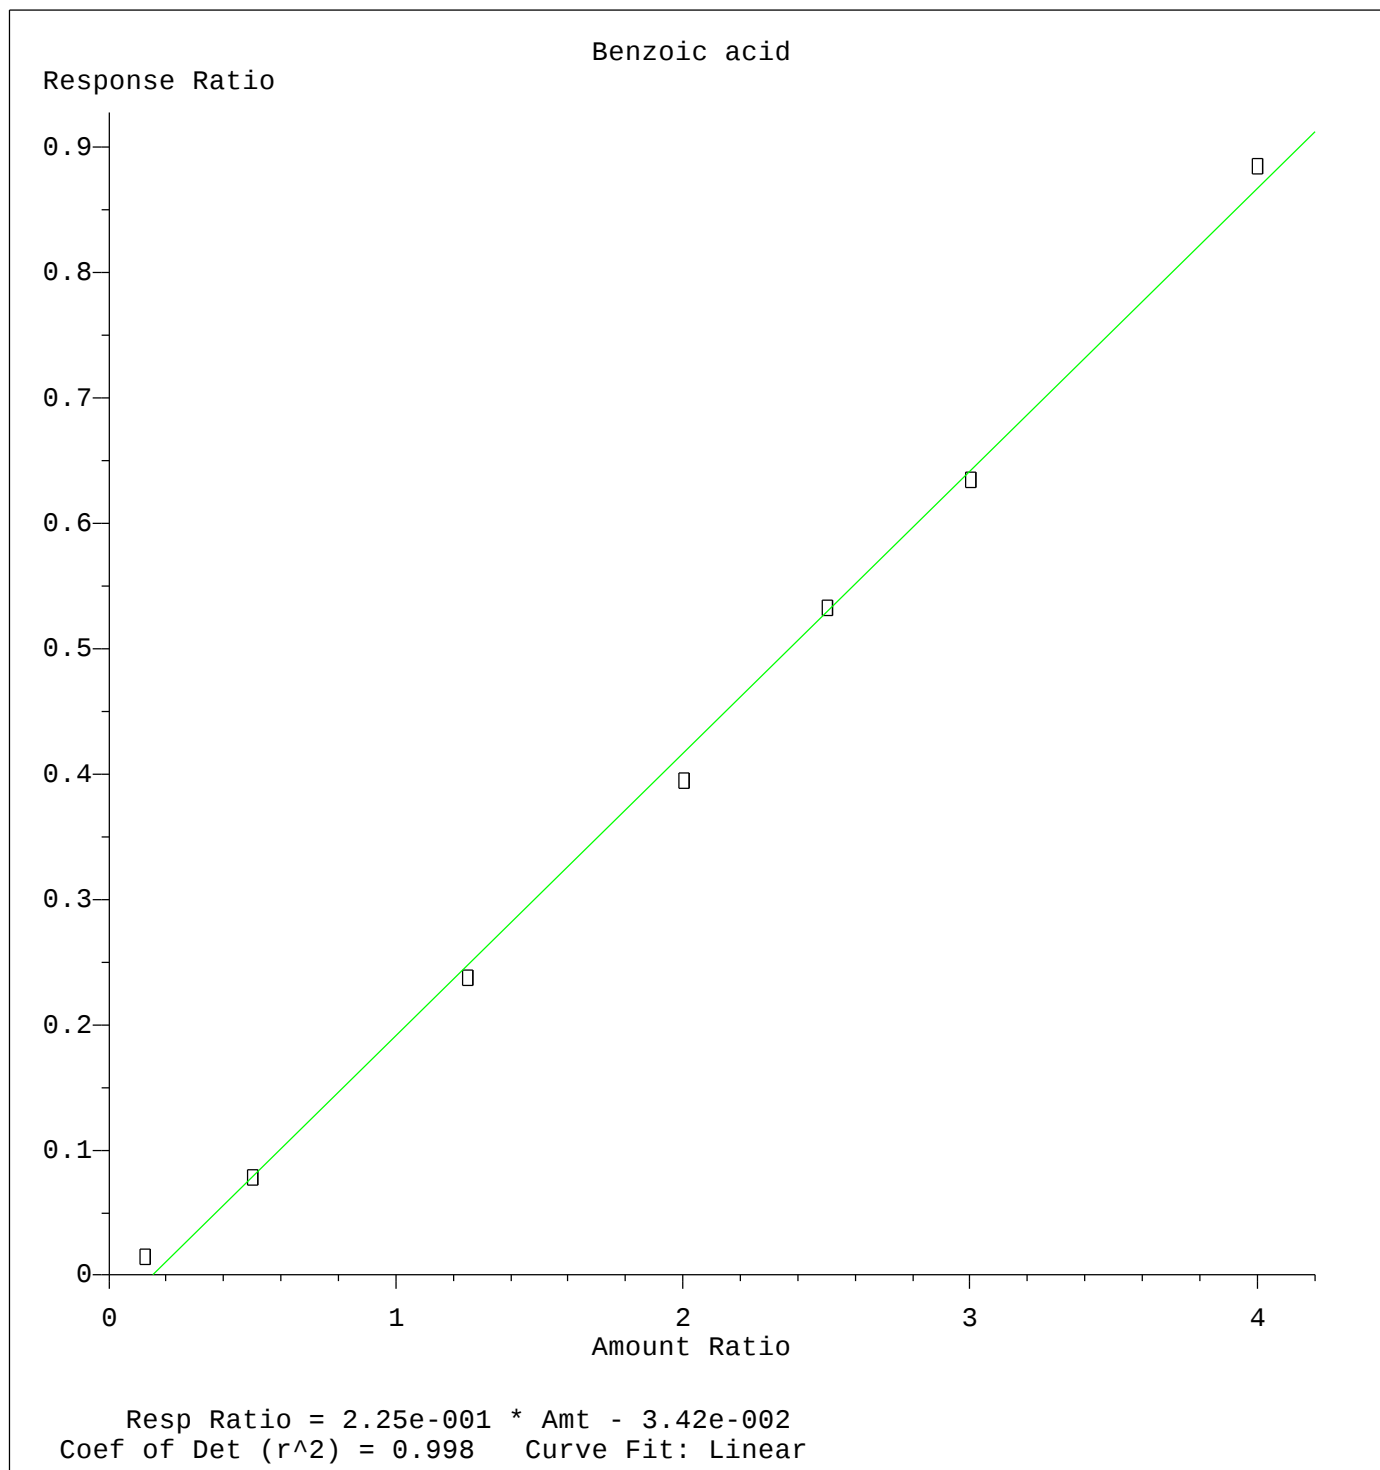

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Calibration Table Last Updated: Wed Dec 09 00:23:35 2015

Hexachlorocyclopentadiene

Response Ratio

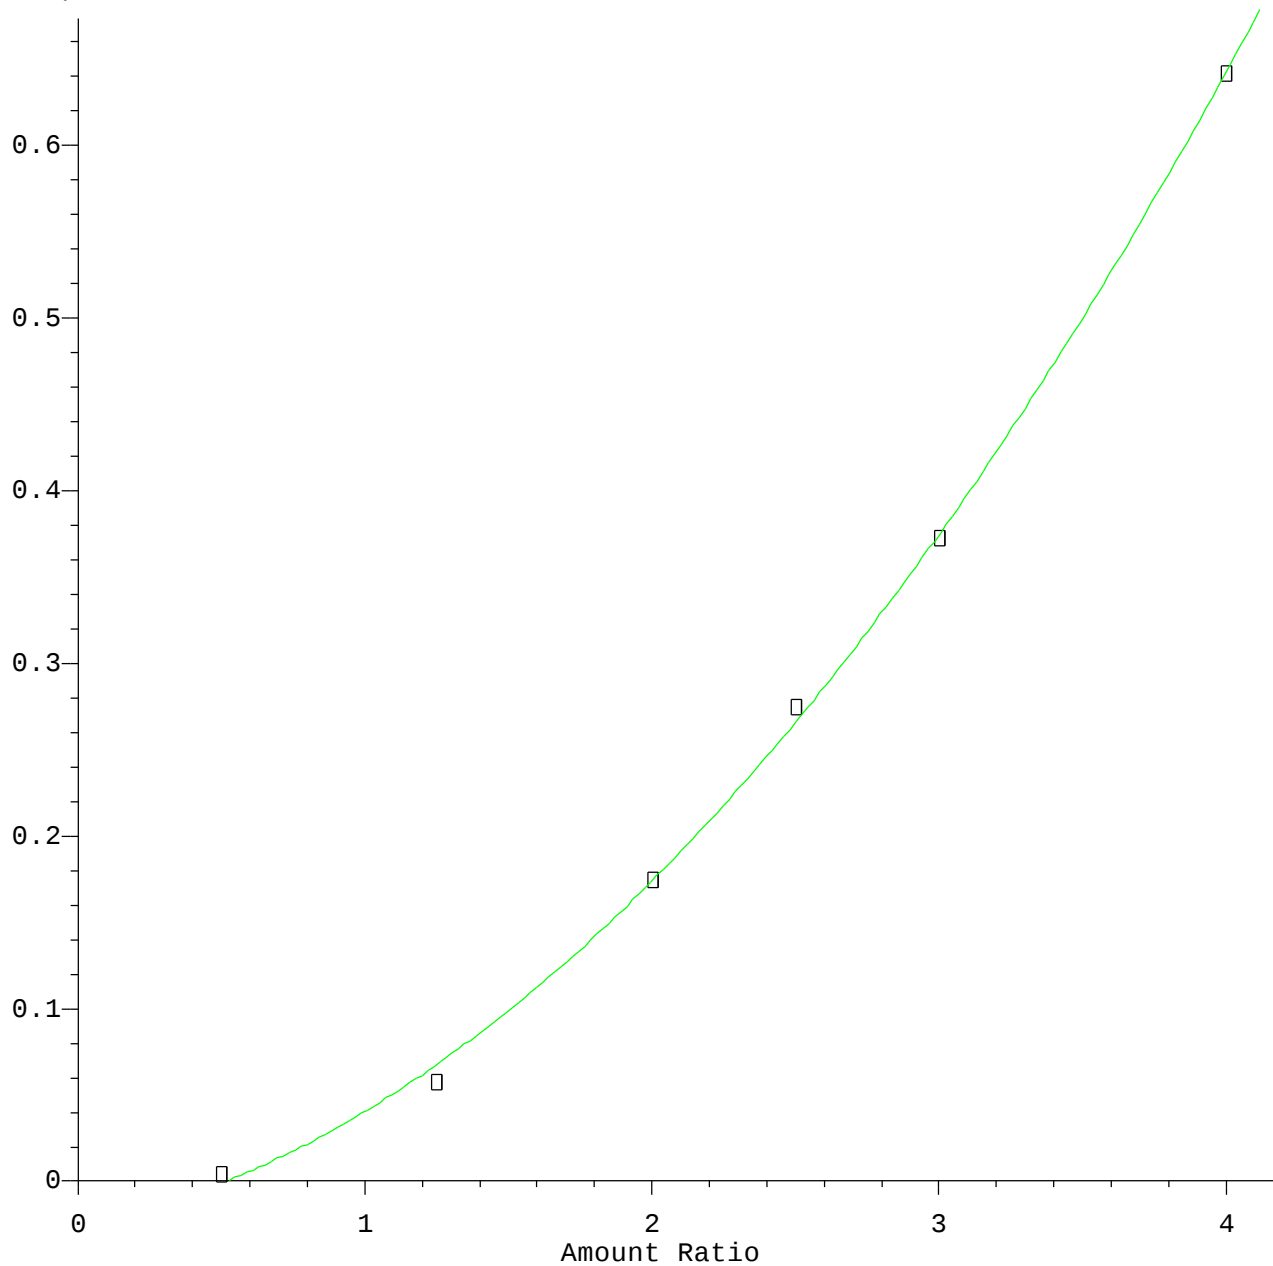


$R = 3.36e-002 A^2 + 3.28e-002 A - 2.61e-002$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Calibration Table Last Updated: Wed Dec 09 00:23:35 2015

2,4-Dinitrophenol

Response Ratio

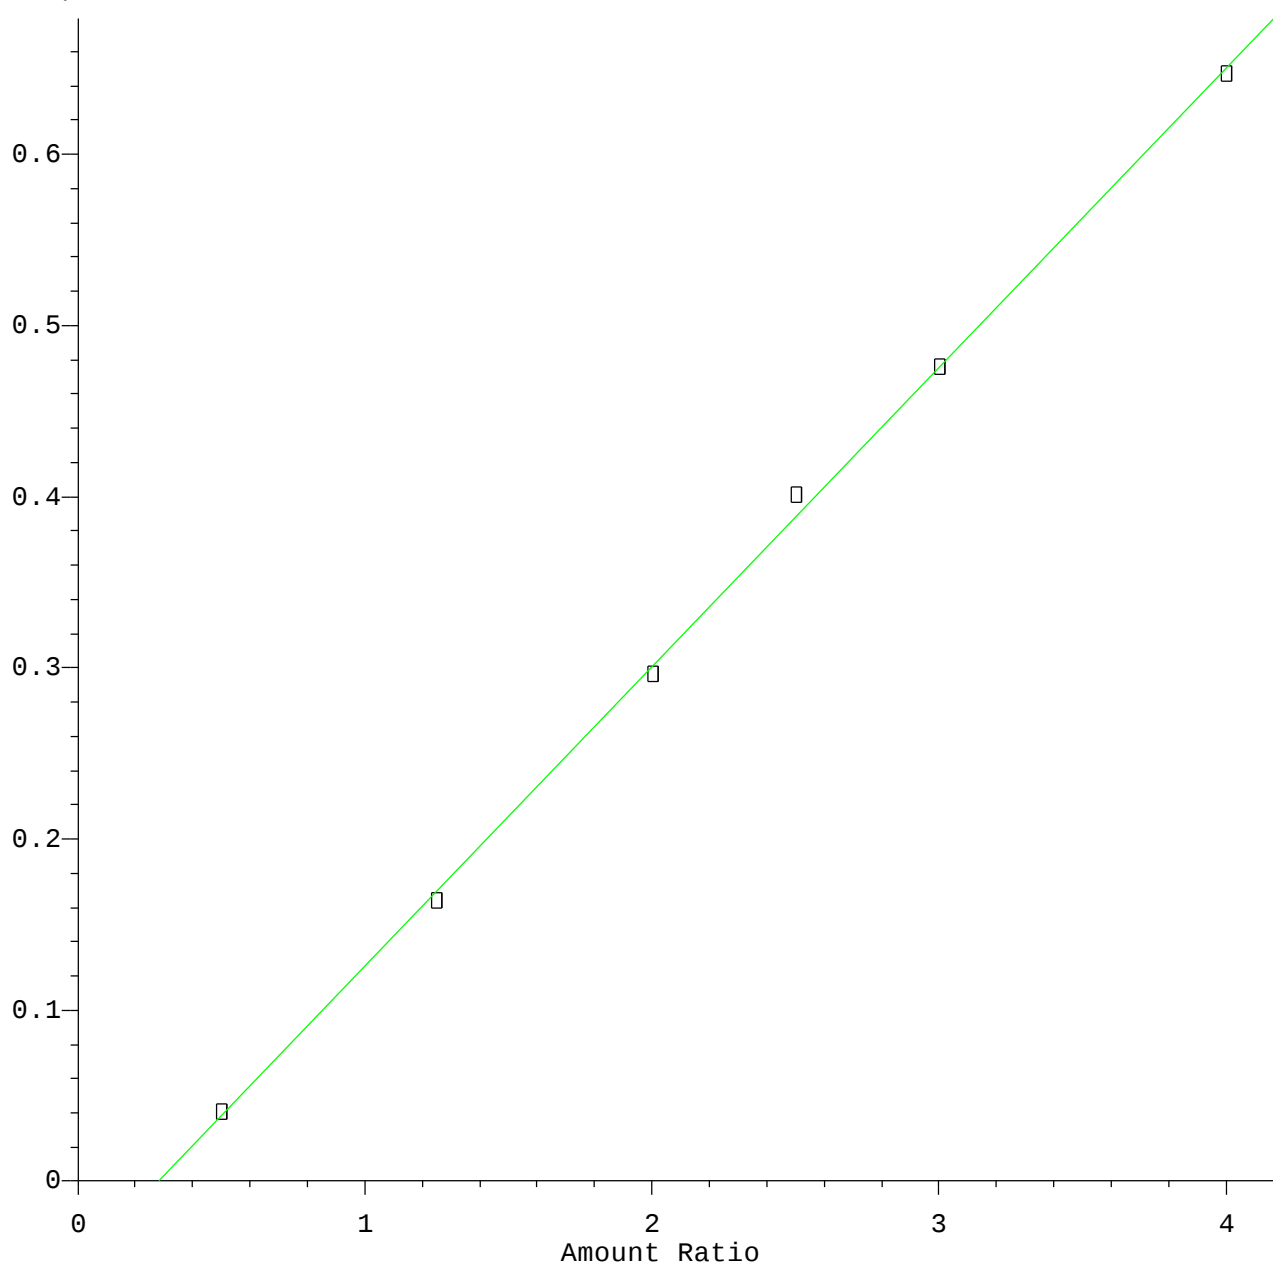


Resp Ratio = 1.75e-001 * Amt - 4.90e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Calibration Table Last Updated: Wed Dec 09 00:23:35 2015

2,3,4,6-Tetrachlorophenol


Response Ratio

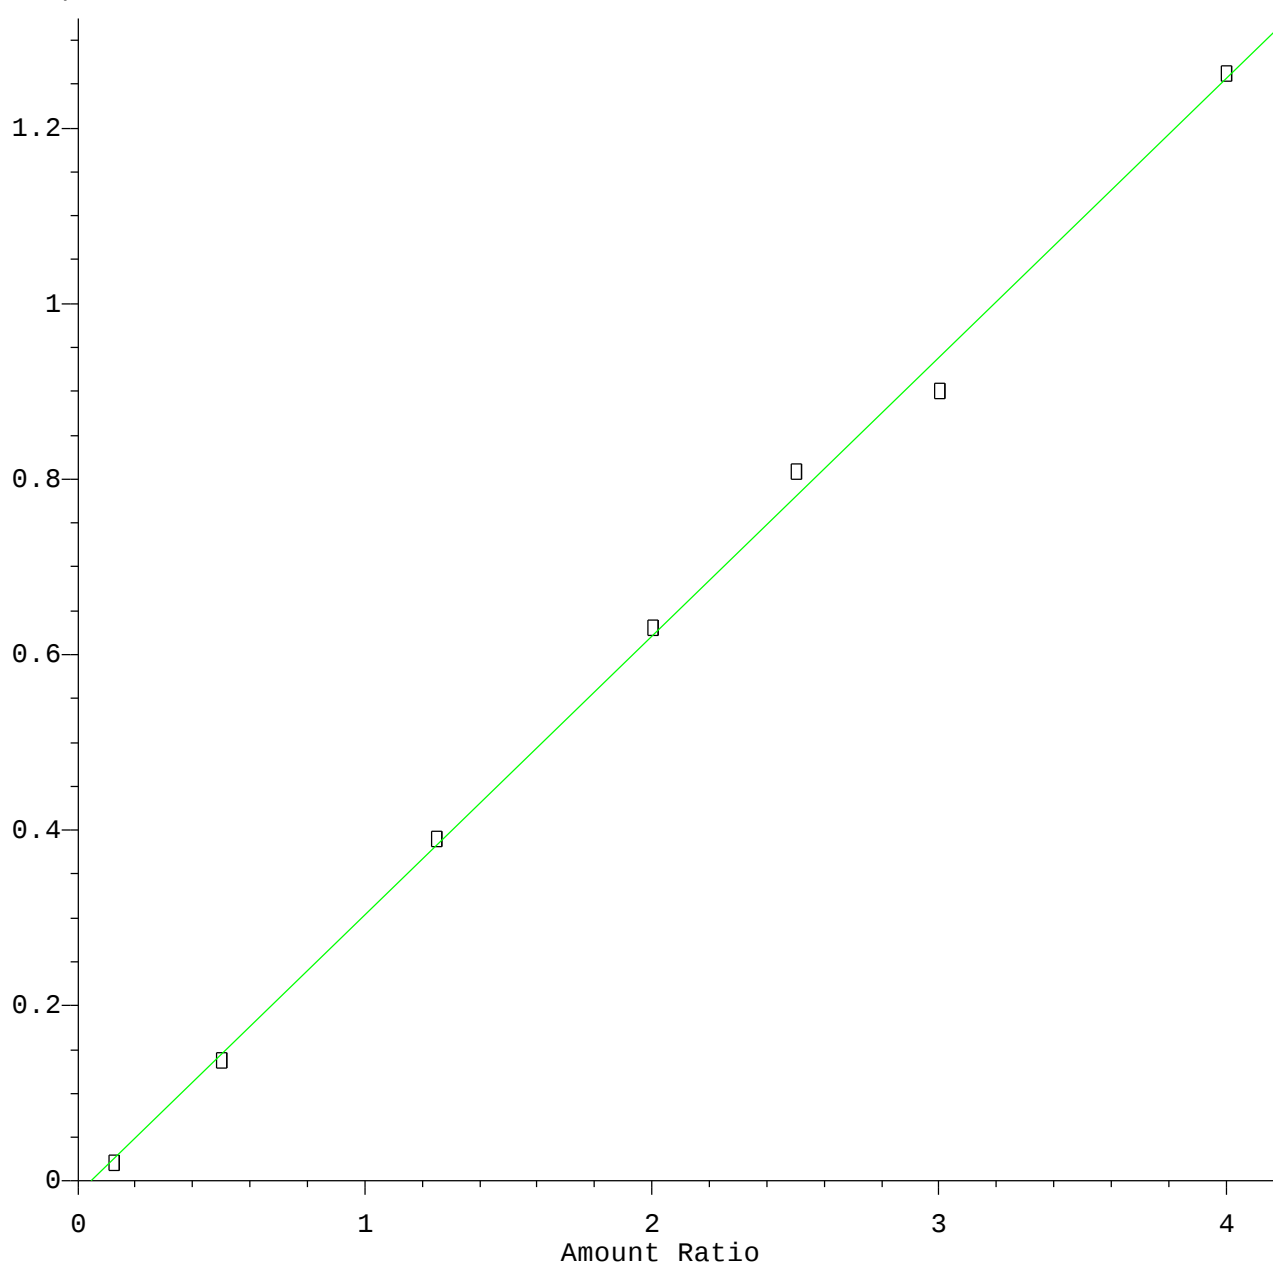

Resp Ratio = $3.18 \times 10^{-1} \times \text{Amt} - 1.46 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Calibration Table Last Updated: Wed Dec 09 00:23:35 2015

4,6-Dinitro-2-methylphenol

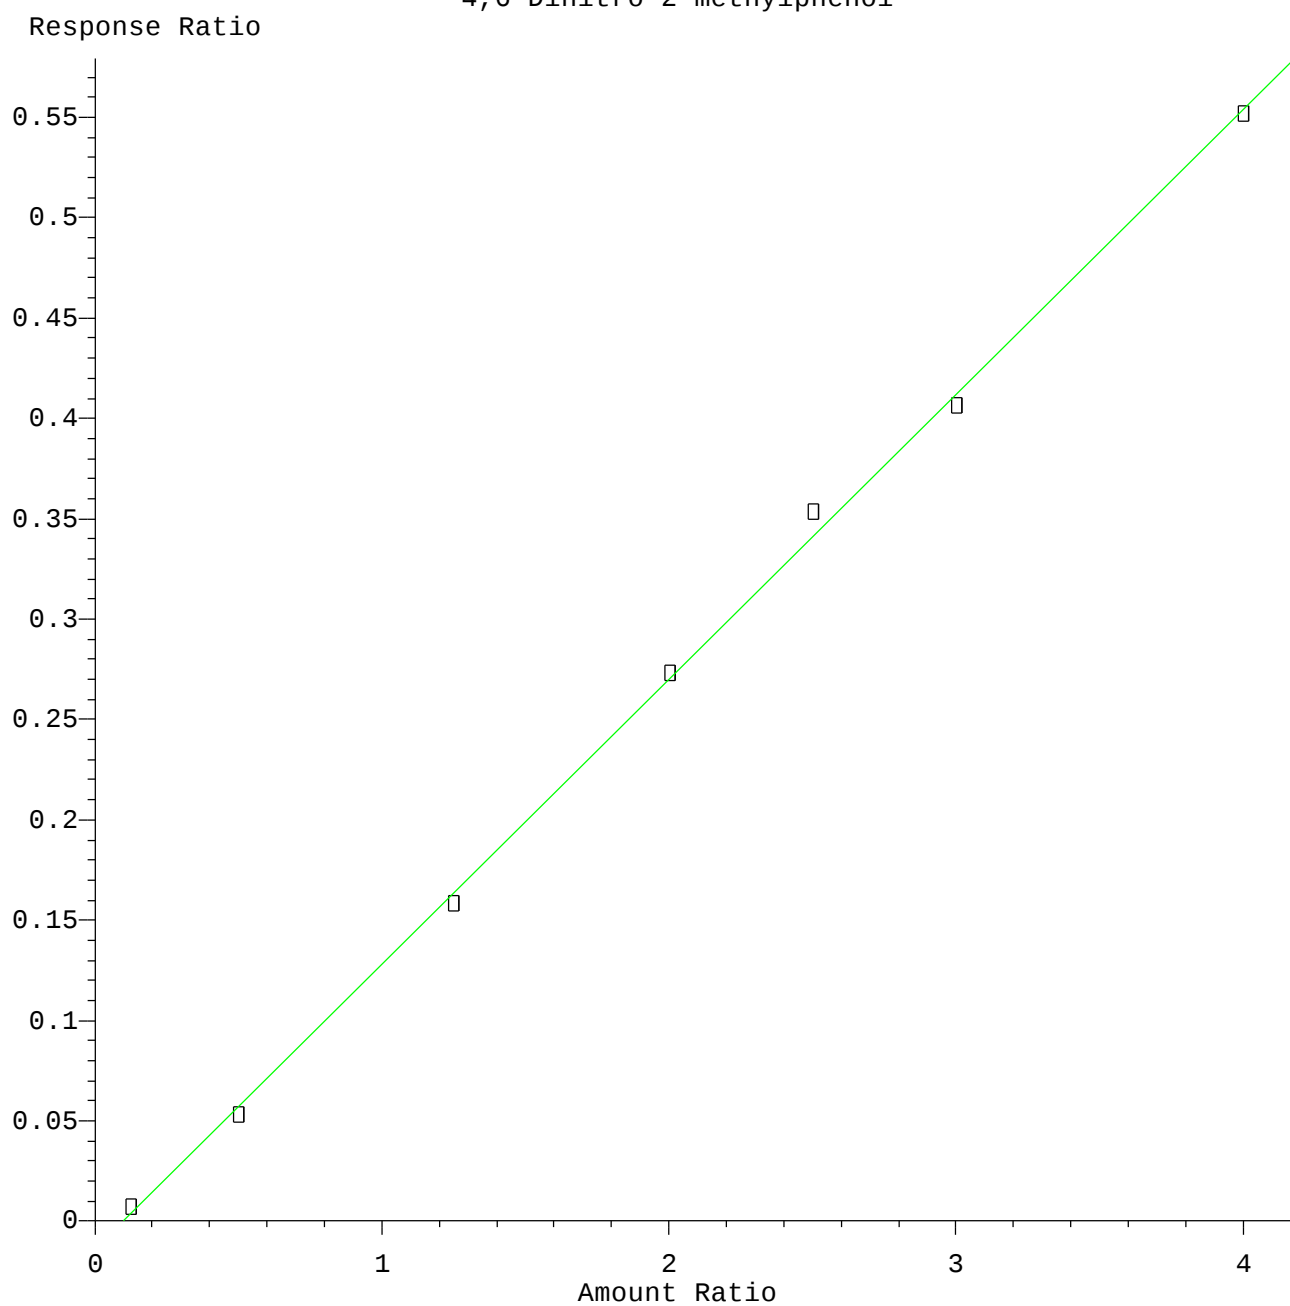

Resp Ratio = $1.42 \times 10^{-1} \times \text{Amt} - 1.38 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Calibration Table Last Updated: Wed Dec 09 00:23:35 2015

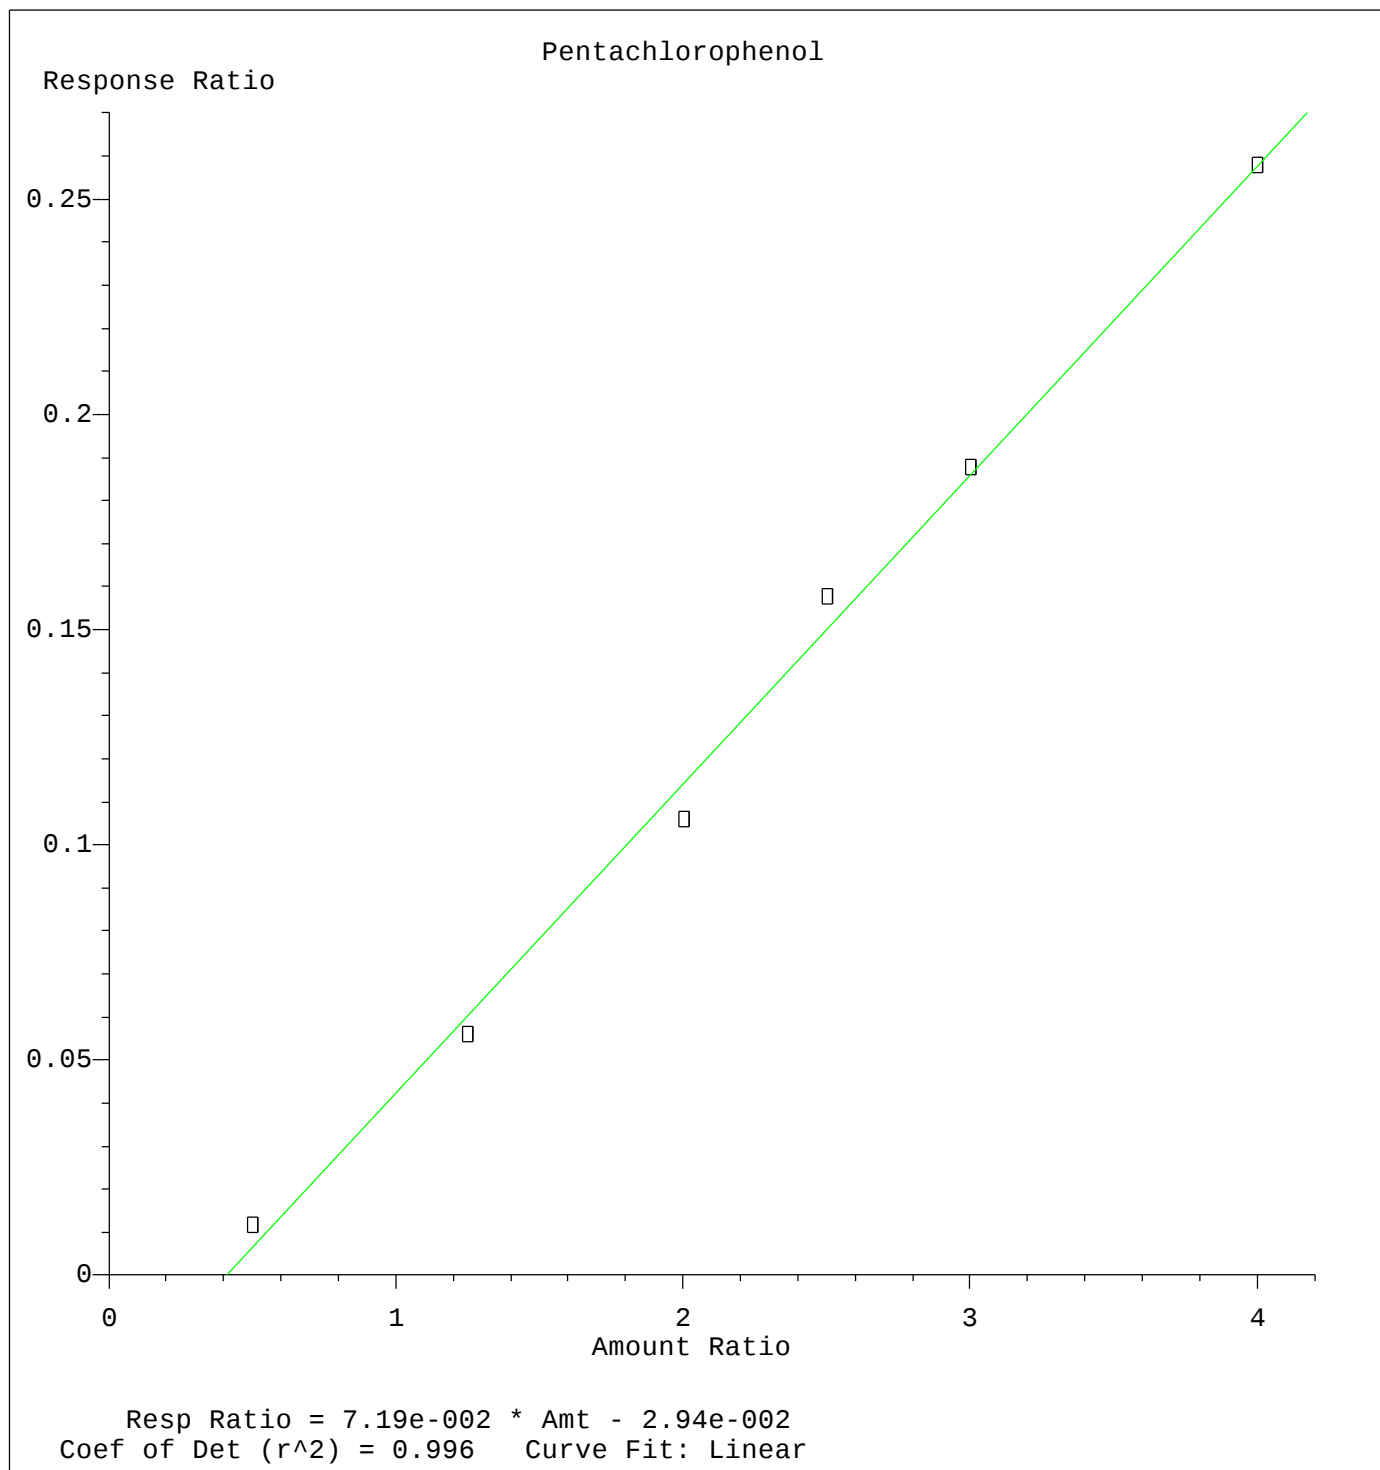

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Calibration Table Last Updated: Wed Dec 09 00:23:35 2015