
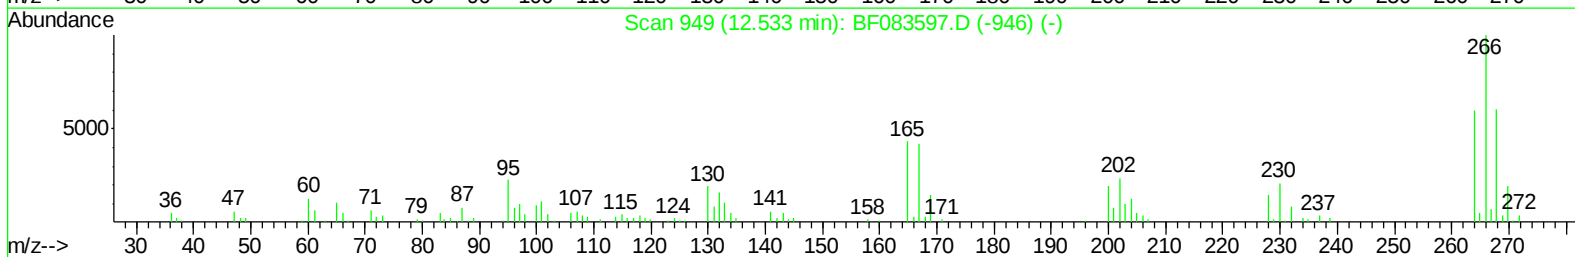
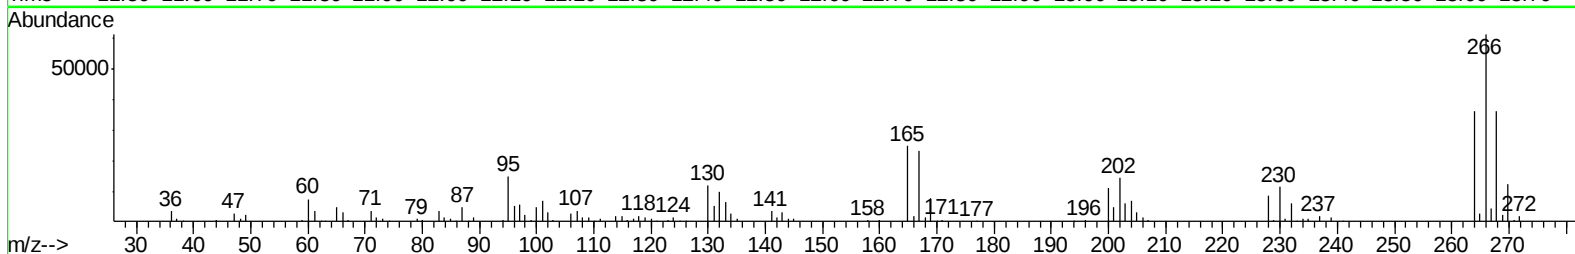


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120815\
Data File : BF083610.D
Acq On : 8 Dec 2015 22:50
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 07:52:45 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 00:23:35 2015
Response via : Initial Calibration

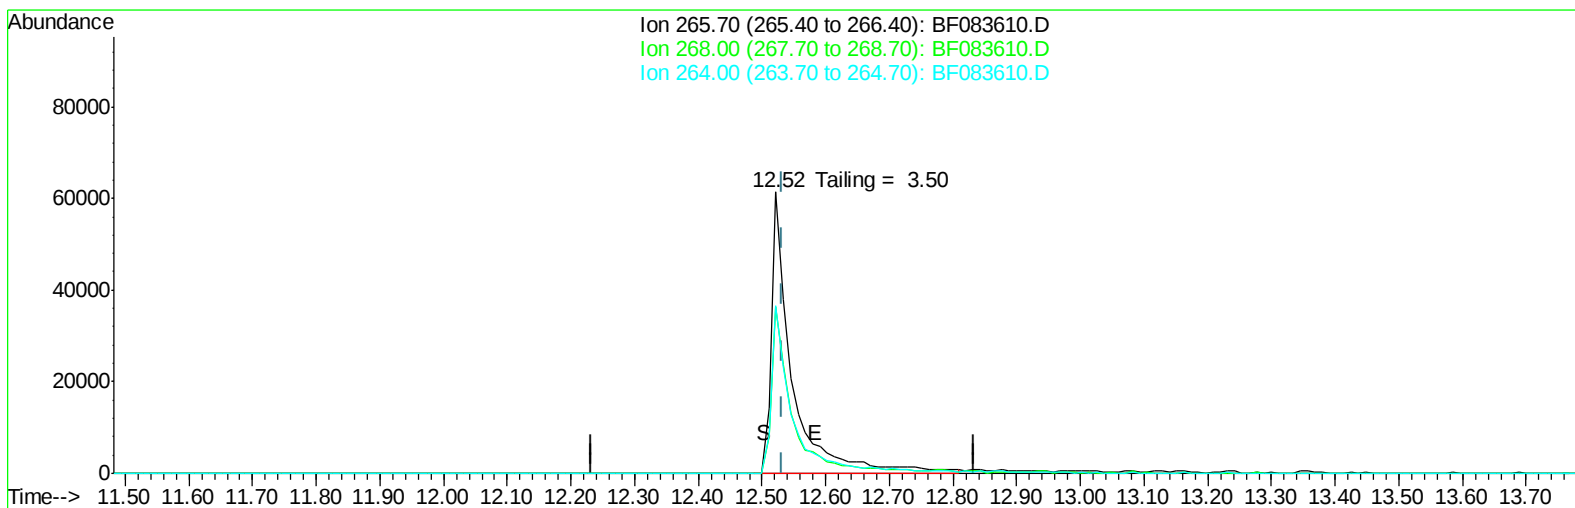

TIC: BF083610.D

(69) Pentachlorophenol (C)




12.522min (-0.011) 0.00ng

response 137827

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	58.97
264.00	64.30	59.34
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF120815\
Data File : BF083610.D
Acq On : 8 Dec 2015 22:50
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 07:52:45 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 00:23:35 2015
Response via : Initial Calibration

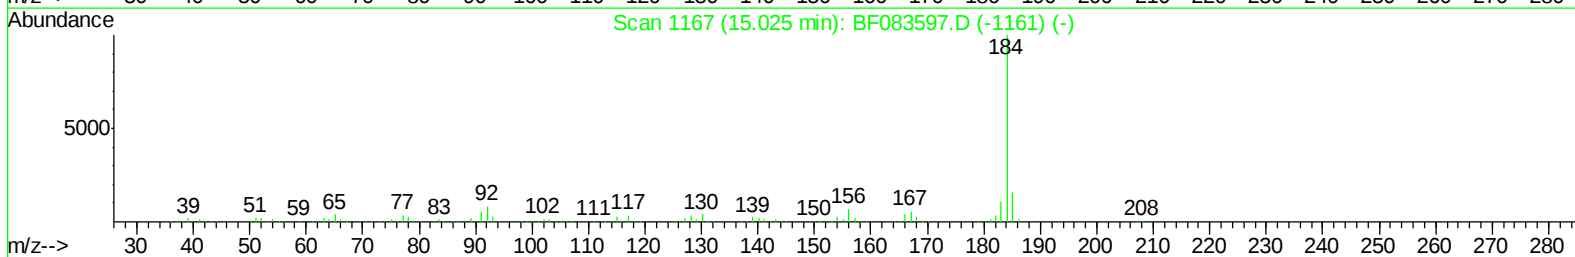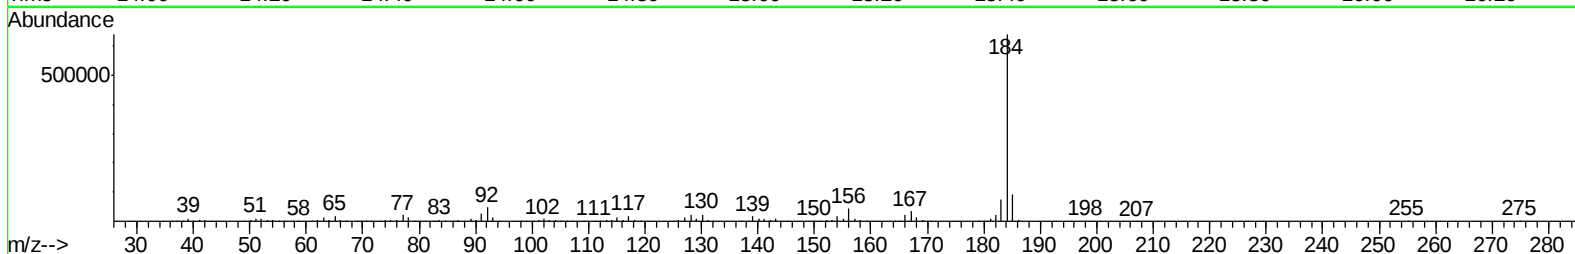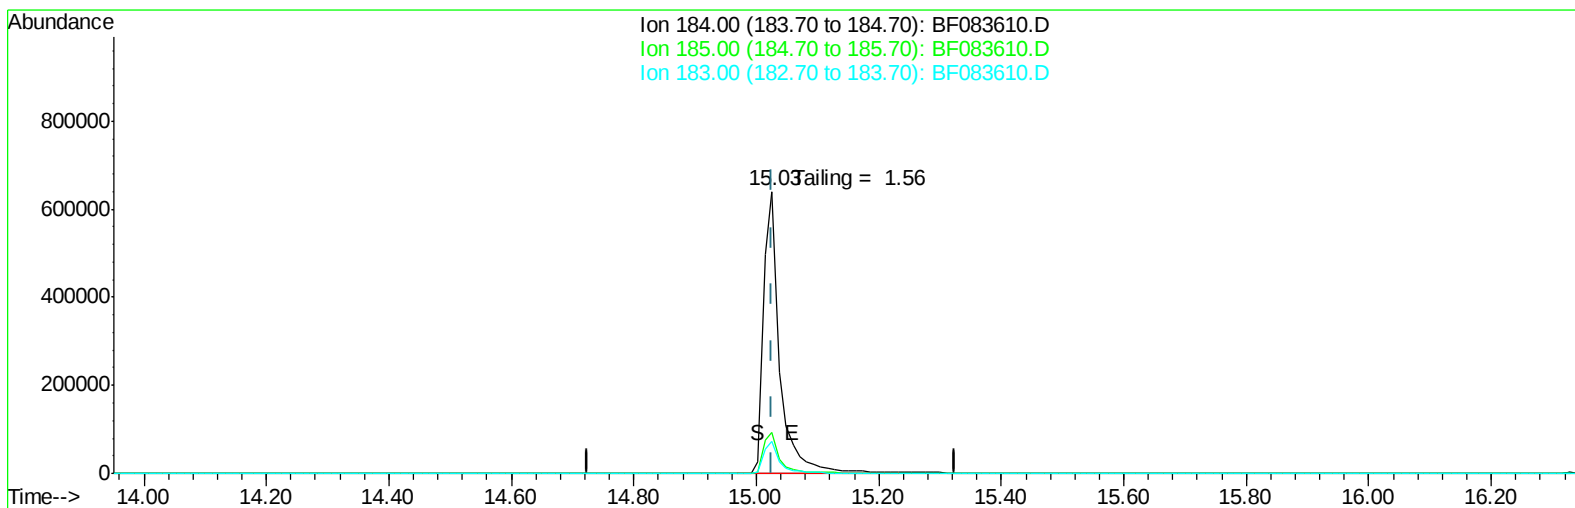

TIC: BF083610.D

(76) Benzidine

15.025min (+0.000) 24499.71ng

response 1194140

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.56
183.00	11.20	11.53
0.00	0.00	0.00