

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120815\
 Data File : BF083606.D
 Acq On : 8 Dec 2015 20:51
 Operator : UM/IZ
 Sample : PB87111BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB87111BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.561	162	164	182	rBV	426747	1152573	21.43%	2.689%
2	3.984	199	201	223	rBV	3347653	4710381	87.59%	10.989%
3	5.264	311	313	322	rBV	3312215	4799015	89.24%	11.196%
4	5.390	322	324	338	rVB	3525235	4770773	88.71%	11.130%
5	5.699	348	351	367	rVB	631386	887658	16.51%	2.071%
6	5.916	367	370	380	rBV	2234013	3611941	67.16%	8.427%
7	6.522	420	423	445	rBV	1932792	3082357	57.32%	7.191%
8	7.596	515	517	533	rBV	711810	1132419	21.06%	2.642%
9	9.333	666	669	688	rBV	2979691	5301147	98.58%	12.368%
10	10.385	758	761	772	rBV	838939	1278320	23.77%	2.982%
11	11.677	871	874	890	rBV	1967861	3108720	57.81%	7.253%
12	12.785	968	971	983	rBV	767093	1319617	24.54%	3.079%
13	15.414	1197	1201	1204	rBV	3743510	5377718	100.00%	12.546%
14	16.991	1336	1339	1356	rBV	813243	1289611	23.98%	3.009%
15	18.637	1480	1483	1498	rBV	504754	1040376	19.35%	2.427%


Sum of corrected areas: 42862626

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120815\
Data File : BF083606.D
Acq On : 8 Dec 2015 20:51
Operator : UM/IZ
Sample : PB87111BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB87111BL

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

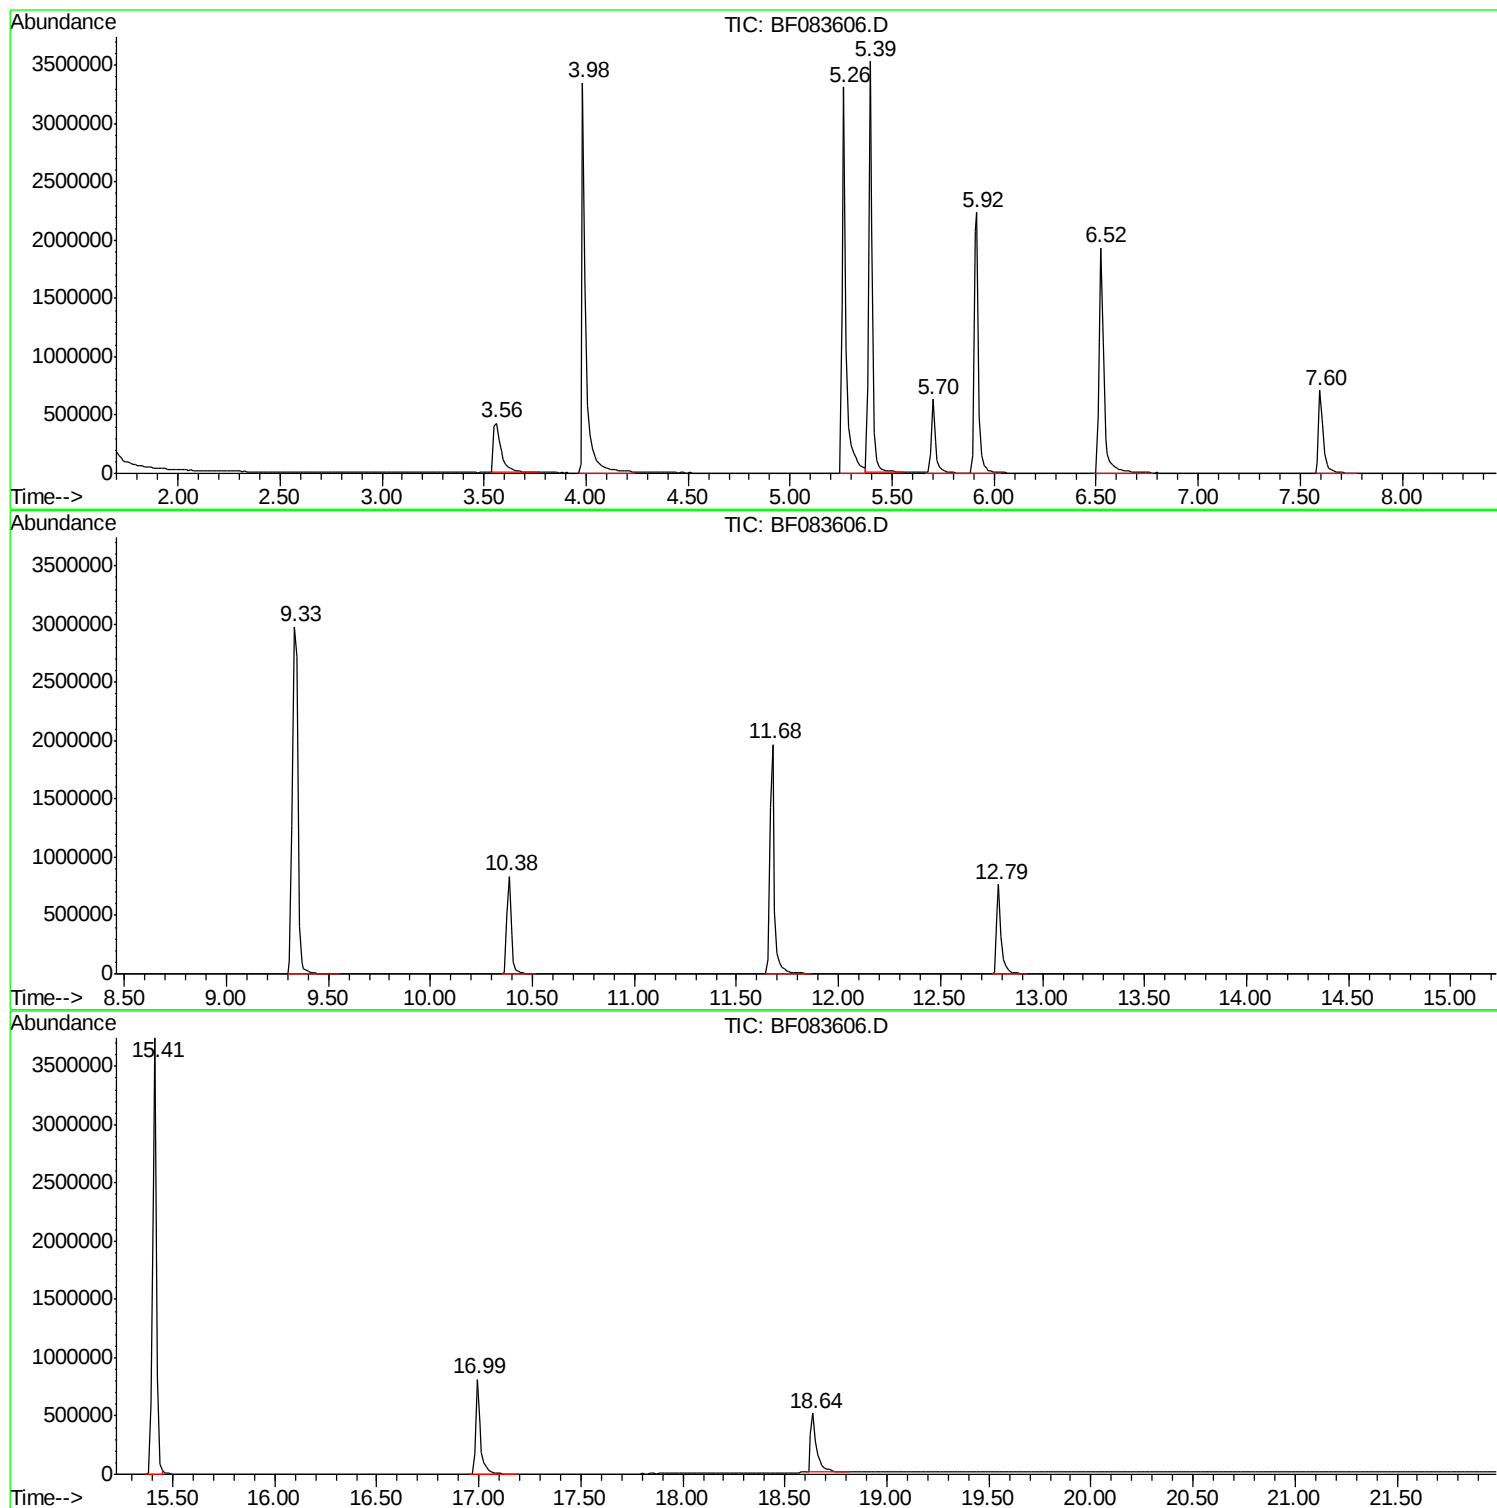

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120815\
Data File : BF083606.D
Acq On : 8 Dec 2015 20:51
Operator : UM/IZ
Sample : PB87111BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB87111BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown3.56 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.56	25.97 ng	1152570	1,4-Dichlorobenzene-d4	5.70

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	33
2			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28
3			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	23
4			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
5			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9

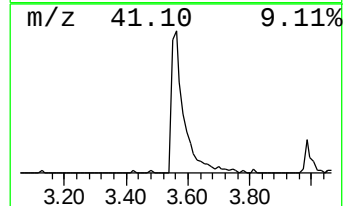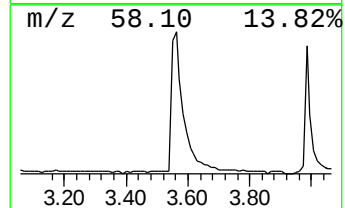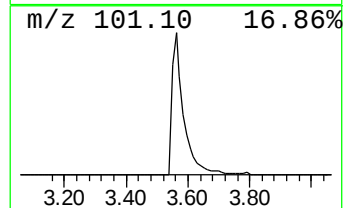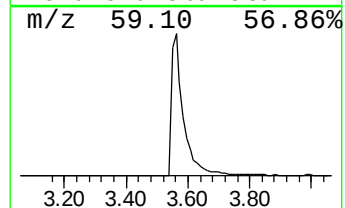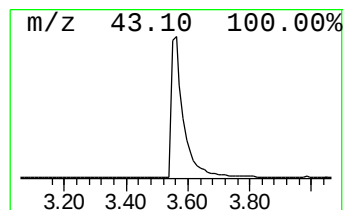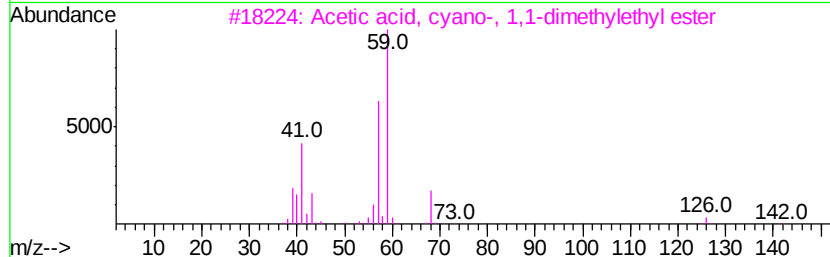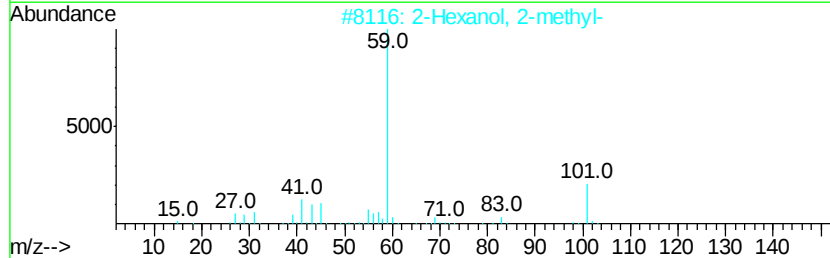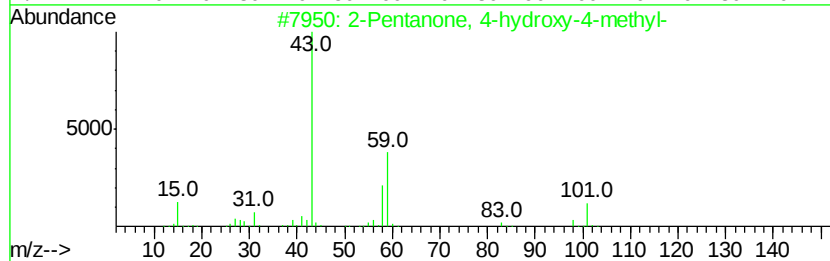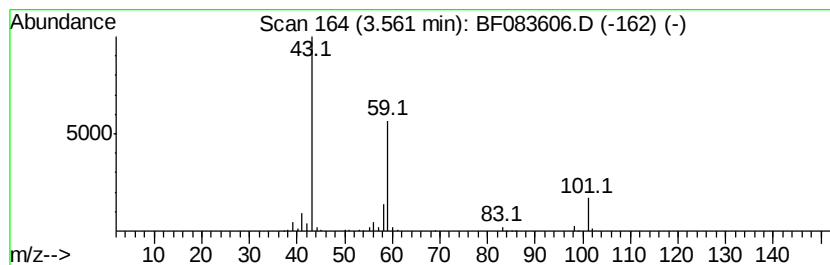

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120815\
Data File : BF083606.D
Acq On : 8 Dec 2015 20:51
Operator : UM/IZ
Sample : PB87111BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB87111BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown5.39 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.39	107.49 ng	4770770	1,4-Dichlorobenzene-d4	5.70

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		2-Cyclohexen-1-one	96	C6H8O	000930-68-7	11
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10

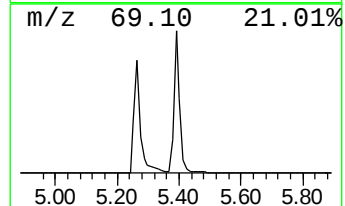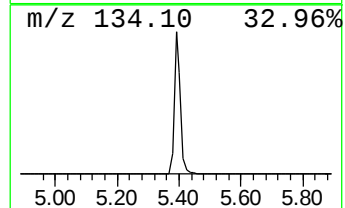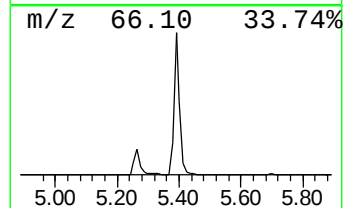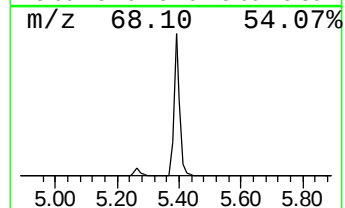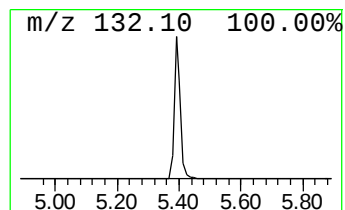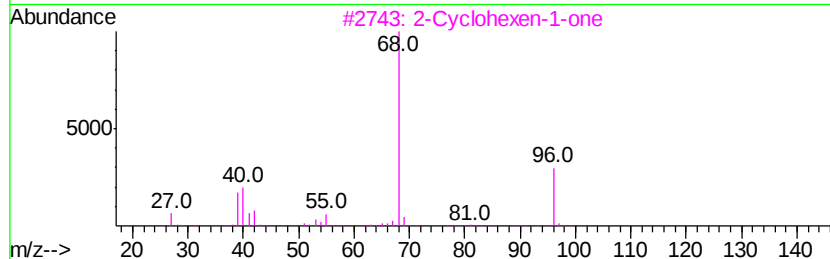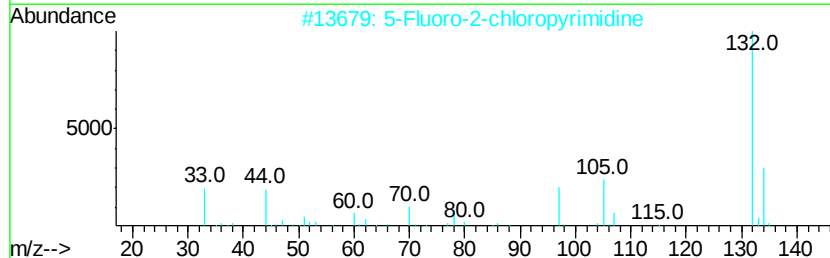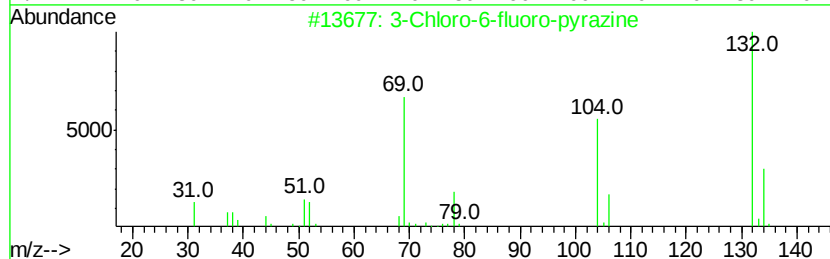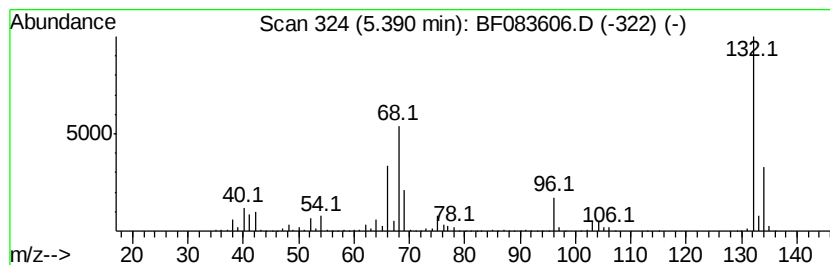

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120815\
Data File : BF083606.D
Acq On : 8 Dec 2015 20:51
Operator : UM/IZ
Sample : PB87111BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB87111BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown3.56	3.56	26.0	ng	1152570	1	5.70	887658	20.0
unknown5.39	5.39	107.5	ng	4770770	1	5.70	887658	20.0