


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120815\
 Data File : BF083592.D
 Acq On : 8 Dec 2015 12:49
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 09 00:23:35 2015

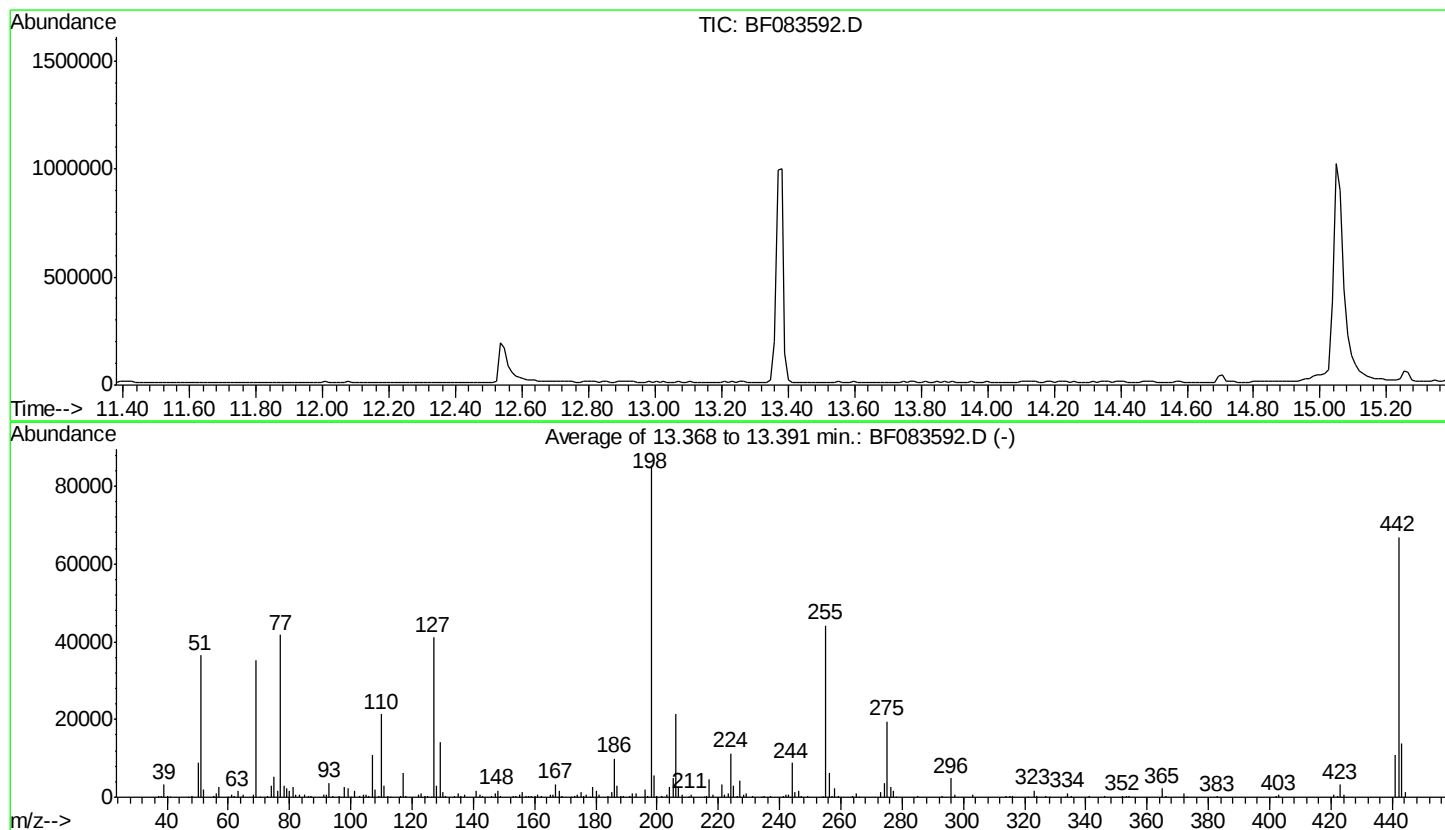

AutoFind: Scans 1022, 1023, 1024; Background Corrected with Scan 1017

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	36509	PASS
68	69	0.00	2	1.6	559	PASS
69	198	0.00	100	41.5	35383	PASS
70	69	0.00	2	0.3	115	PASS
127	198	10	80	48.1	41016	PASS
197	198	0.00	2	0.6	470	PASS
198	198	100	100	100.0	85289	PASS
199	198	5	9	6.6	5617	PASS
275	198	10	60	22.9	19559	PASS
365	198	1	100	2.5	2161	PASS
441	442	0.01	24	16.4	10987	PASS
442	198	50	100	78.4	66853	PASS
443	442	15	24	20.6	13767	PASS