


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120815\
Data File : BF083610.D
Acq On : 8 Dec 2015 22:50
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 09 00:23:35 2015

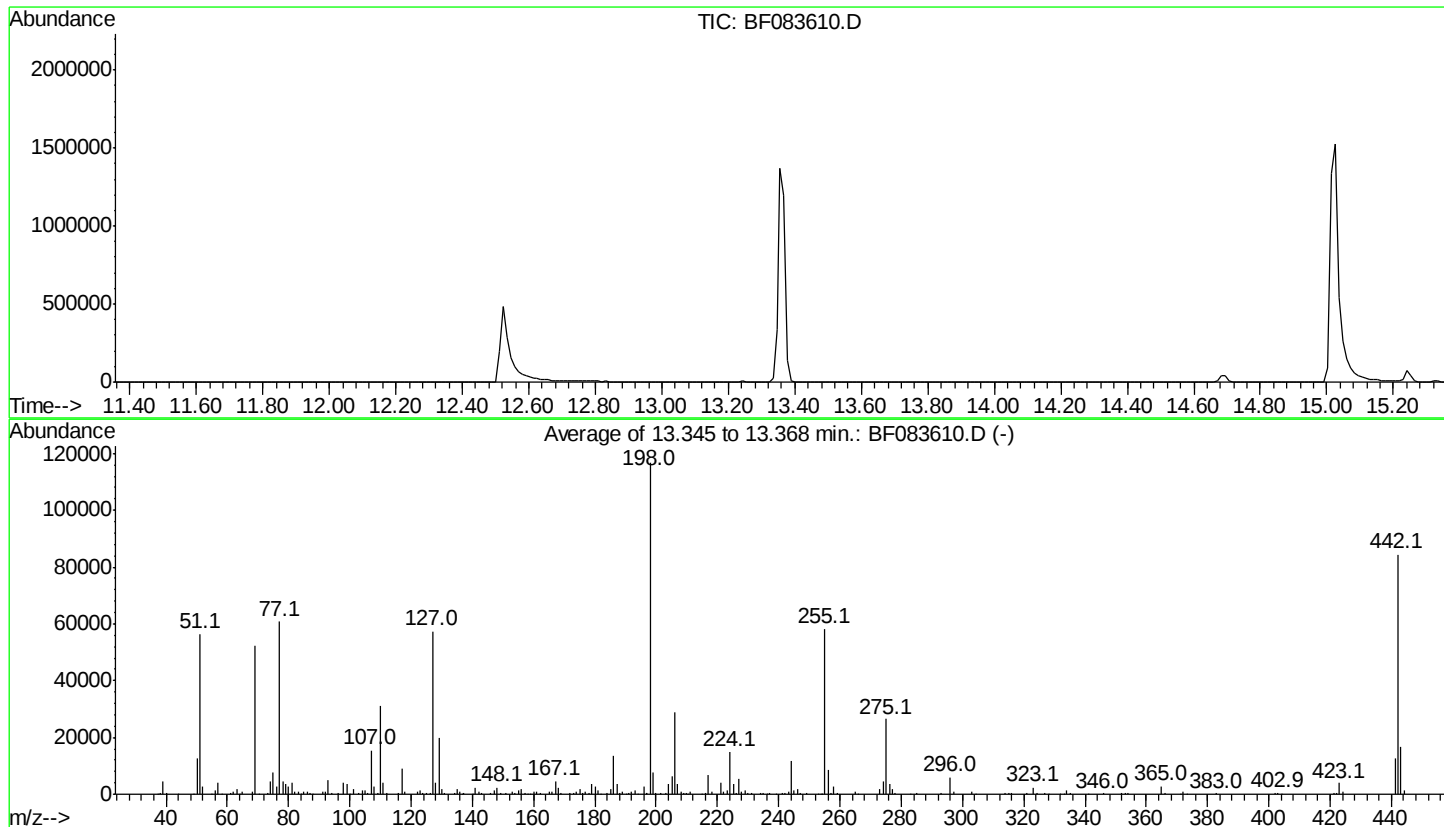

AutoFind: Scans 1020, 1021, 1022; Background Corrected with Scan 1016

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	56456	PASS
68	69	0.00	2	1.6	814	PASS
69	198	0.00	100	44.7	52160	PASS
70	69	0.00	2	0.3	140	PASS
127	198	10	80	49.1	57296	PASS
197	198	0.00	2	0.5	597	PASS
198	198	100	100	100.0	116760	PASS
199	198	5	9	6.7	7835	PASS
275	198	10	60	22.7	26471	PASS
365	198	1	100	2.4	2801	PASS
441	442	0.01	24	14.9	12536	PASS
442	198	50	100	72.3	84367	PASS
443	442	15	24	19.5	16480	PASS