


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120816\
 Data File : BF091502.D
 Acq On : 8 Dec 2016 14:05
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 13:33:46 2016

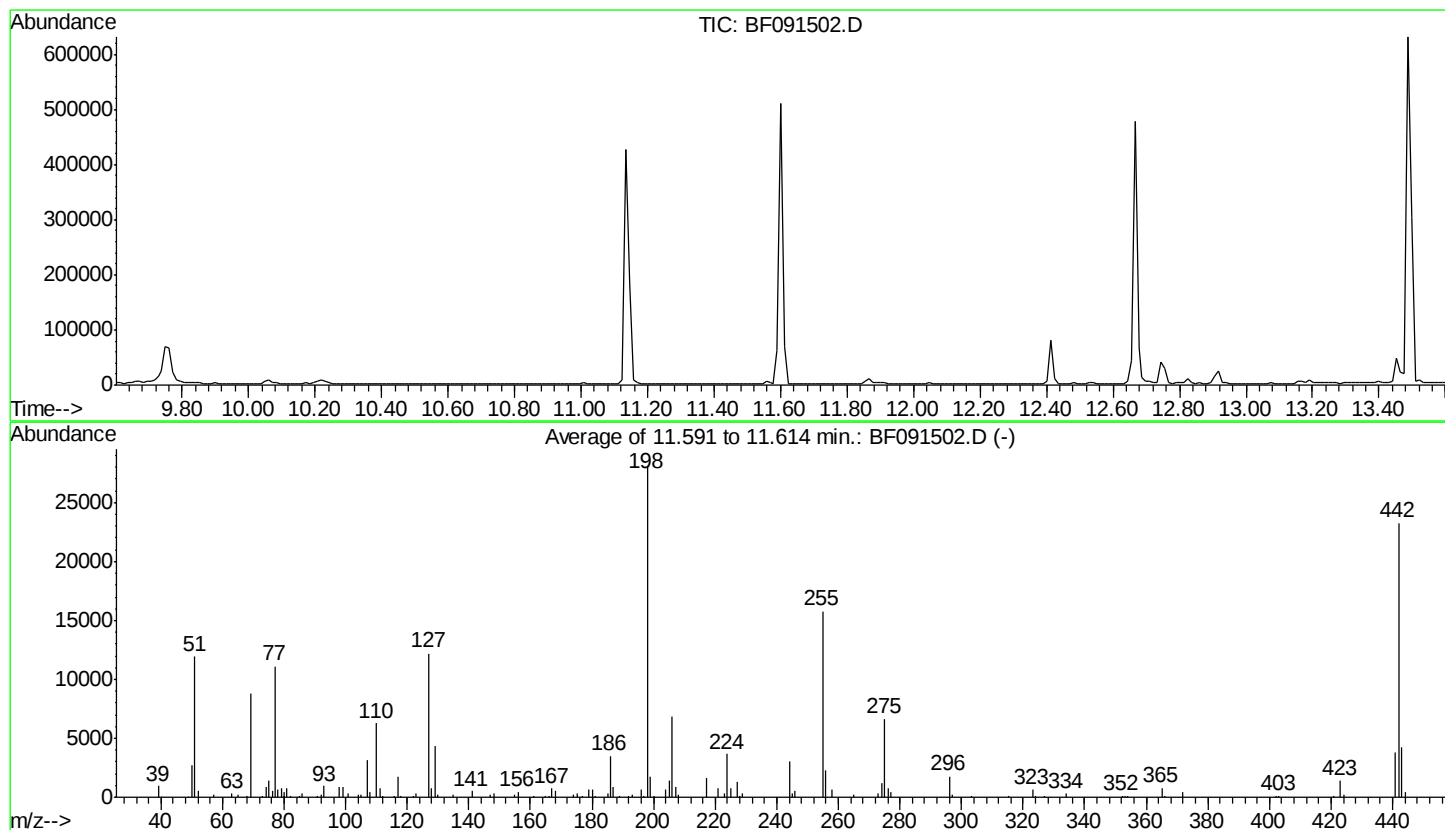

AutoFind: Scans 814, 815, 816; Background Corrected with Scan 811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	11937	PASS
68	69	0.00	2	1.8	160	PASS
69	198	0.00	100	31.4	8829	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.3	12193	PASS
197	198	0.00	2	0.6	165	PASS
198	198	100	100	100.0	28134	PASS
199	198	5	9	6.2	1739	PASS
275	198	10	60	23.6	6646	PASS
365	198	1	100	2.8	789	PASS
441	442	0.01	24	16.3	3803	PASS
442	198	50	100	82.8	23283	PASS
443	442	15	24	18.4	4286	PASS