

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF120817\
 Data File : BF101240.D
 Acq On : 8 Dec 2017 17:17
 Operator : SJ/JU
 Sample : I6680-03 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Dec 08 18:19:39 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 08 18:17:31 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	43020	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	174226	20.00	ng	0.00
38) Acenaphthene-d10	9.86	164	77260	20.00	ng	0.00
63) Phenanthrene-d10	11.35	188	136172	20.00	ng	0.00
75) Chrysene-d12	14.00	240	99460	20.00	ng	0.00
86) Perylene-d12	15.46	264	91737	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.43	112	23158	8.90	ng	0.00
7) Phenol-d6	6.45	99	27889	8.82	ng	-0.01
23) Nitrobenzene-d5	7.39	82	16616	5.69	ng	-0.01
41) 2,4,6-Tribromophenol	10.65	330	6917	7.45	ng	-0.01
44) 2-Fluorobiphenyl	9.18	172	40715	7.21	ng	0.00
78) Terphenyl-d14	12.93	244	33055	7.27	ng	0.00
Target Compounds						
25) Isophorone	7.39	82	16616	3.331	ng	# 64
50) 2,6-Dinitrotoluene	9.86	165	9979	7.604	ng	# 24
56) 2,4-Dinitrotoluene	9.86	165	9979	5.674	ng	# 21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF120817\
Data File : BF101240.D
Acq On : 8 Dec 2017 17:17
Operator : SJ/JU
Sample : I6680-03 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :

Quant Time: Dec 08 18:19:39 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 08 18:17:31 2017
Response via : Initial Calibration

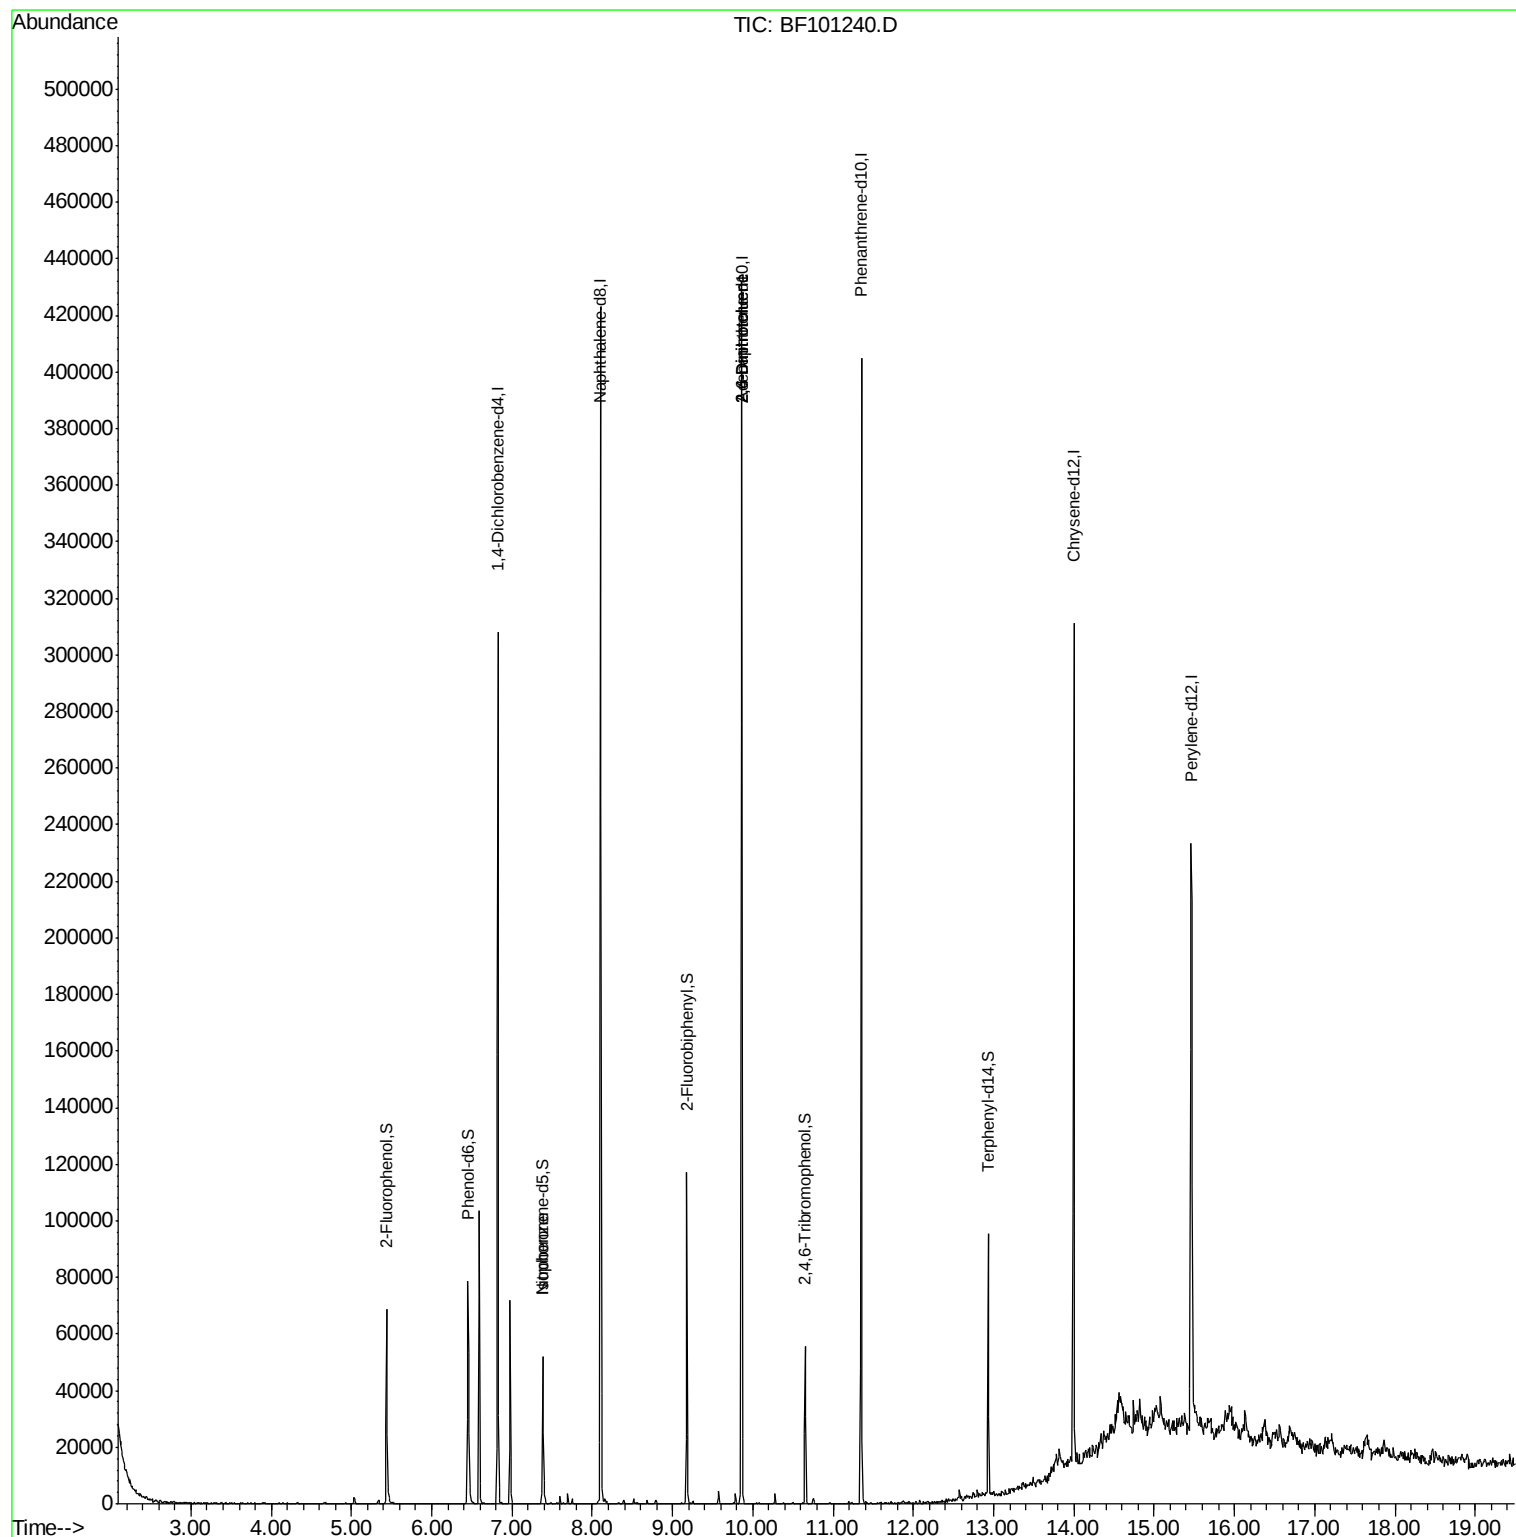

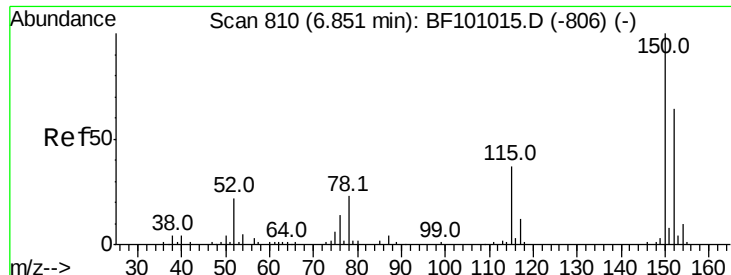


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.82 min Scan# 805
Delta R.T. -0.00 min
Lab File: BF101240.D
Acq: 8 Dec 2017 17:17

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 43020
Ion Ratio Lower Upper
152 100
150 160.9 124.6 186.8
115 60.1 50.1 75.1

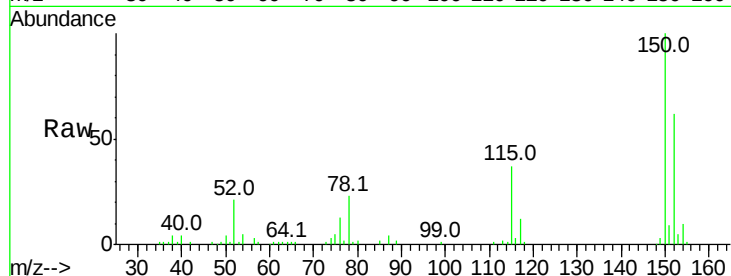


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

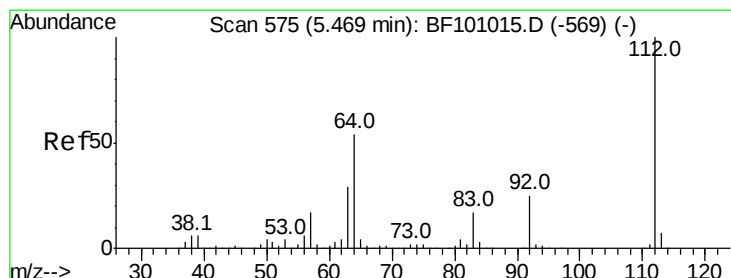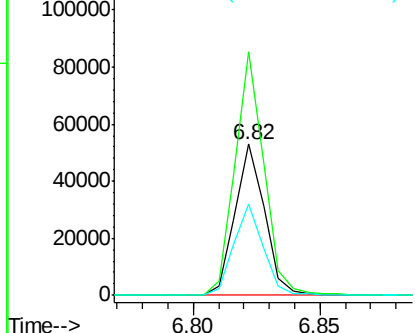



#5


2-Fluorophenol
Concen: 8.895 ng
RT: 5.43 min Scan# 569
Delta R.T. -0.01 min
Lab File: BF101240.D
Acq: 8 Dec 2017 17:17

Tgt Ion:112 Resp: 23158
Ion Ratio Lower Upper
112 100
64 59.4 47.9 71.9
63 31.4 23.7 35.5

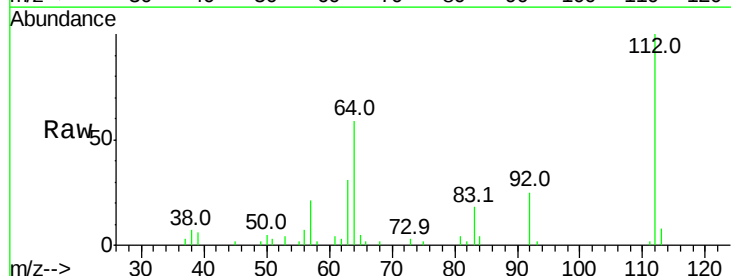

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

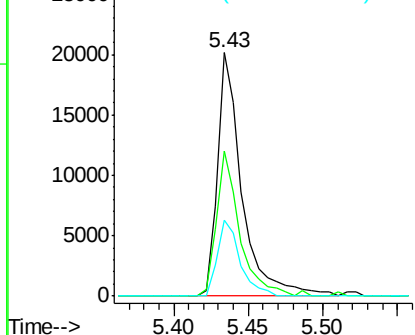

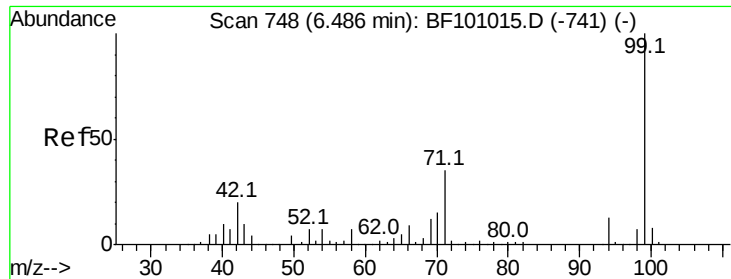

#7

Phenol-d6

Concen: 8.823 ng

RT: 6.45 min Scan# 742

Delta R.T. -0.01 min

Lab File: BF101240.D

Acq: 8 Dec 2017 17:17

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 27889

Ion Ratio Lower Upper




99 100

42 19.8 14.5 21.7

71 34.4 25.4 38.0

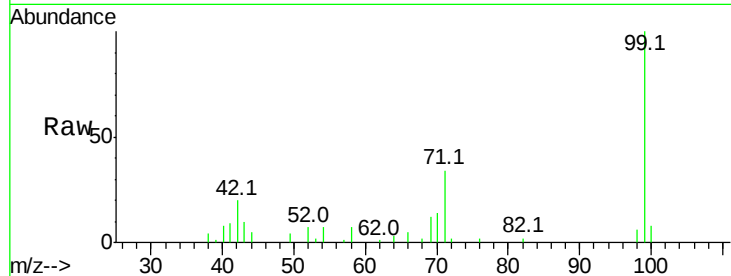

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

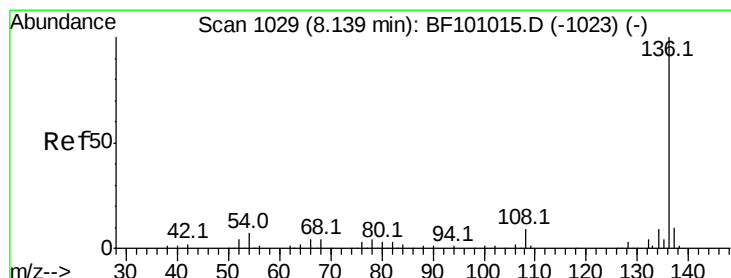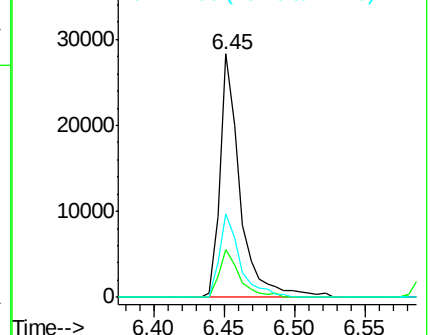

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1023

Delta R.T. -0.01 min

Lab File: BF101240.D

Acq: 8 Dec 2017 17:17

Tgt Ion: 136 Resp: 174226


Ion Ratio Lower Upper

136 100



137 10.9 8.9 13.3


54 6.9 6.6 9.8

68 4.7 5.0 7.4#

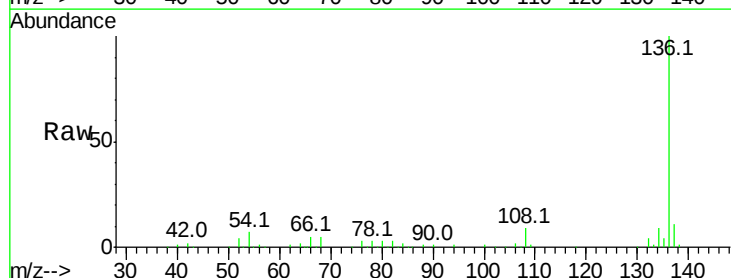

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

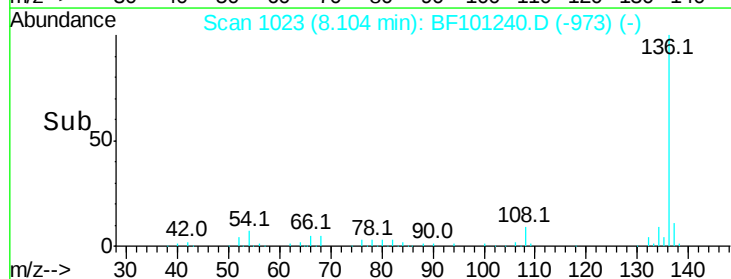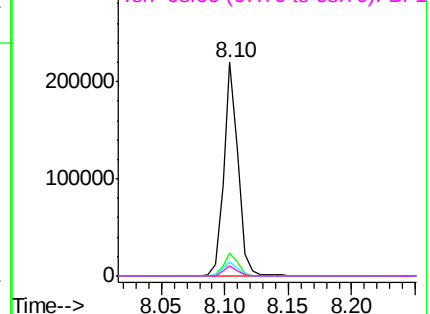


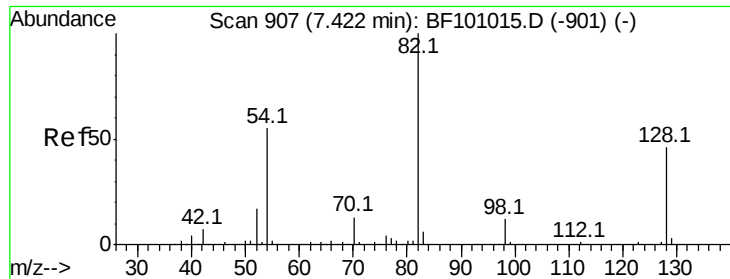




#23
Nitrobenzene-d5
Concen: 5.689 ng
RT: 7.39 min Scan# 901
Delta R.T. -0.01 min
Lab File: BF101240.D
Acq: 8 Dec 2017 17:17

Instrument :
BNA_F
ClientSampleId :

Tot Ion	82	Resp	16616
Ion Ratio	Lower	Upper	
82	100		
128	50.0	36.1	54.1
54	60.4	41.4	62.2

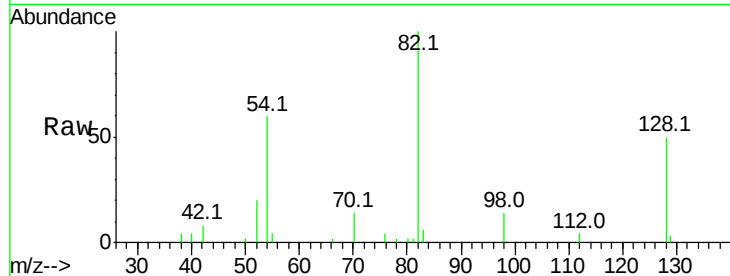


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

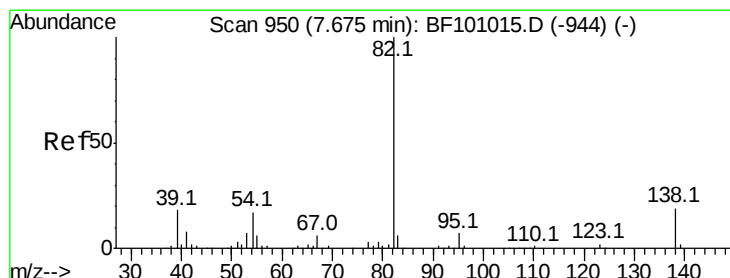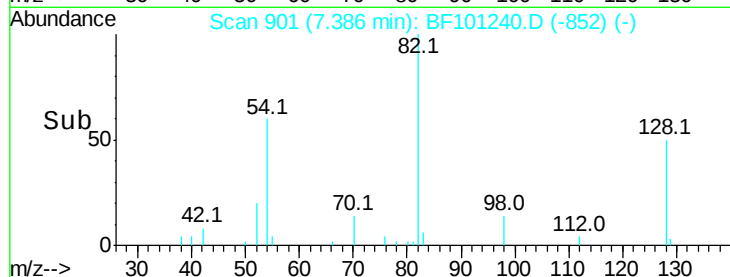
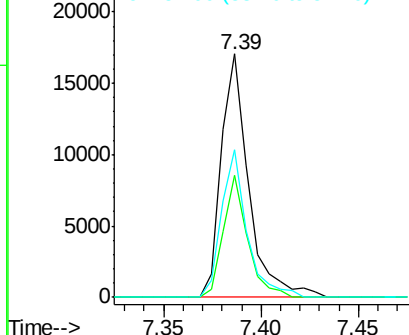



#25
Isophorone
Concen: 3.331 ng
RT: 7.39 min Scan# 901
Delta R.T. -0.26 min
Lab File: BF101240.D
Acq: 8 Dec 2017 17:17

Tgt Ion	82	Resp	16616
Ion Ratio	Lower	Upper	
82	100		
95	0.0	5.2	7.8#
138	0.0	14.9	22.3#

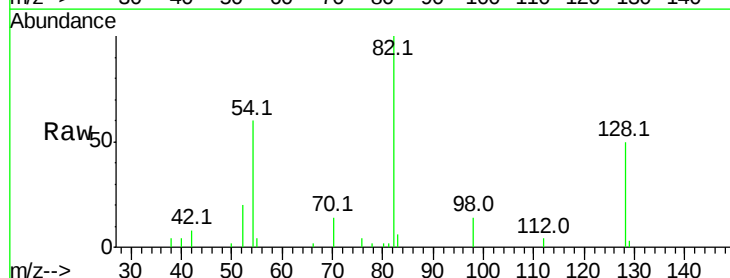

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

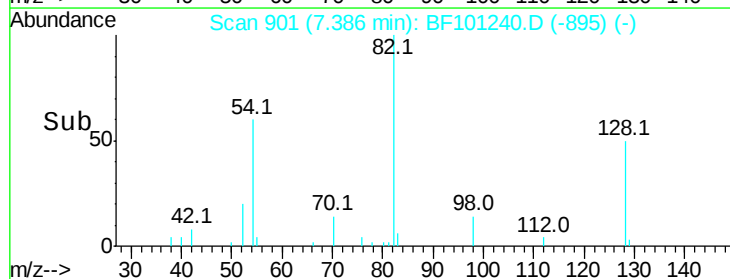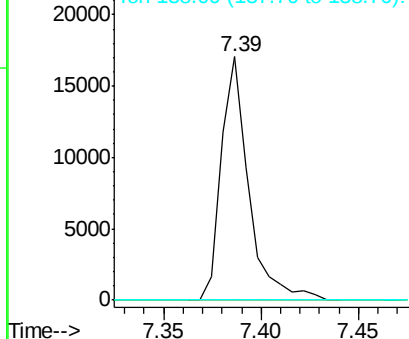







#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.86 min Scan# 1322
 Delta R.T. -0.01 min
 Lab File: BF101240.D
 Acq: 8 Dec 2017 17:17

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:164 Resp: 77260
 Ion Ratio Lower Upper
 164 100
 162 103.6 86.1 129.1
 160 47.2 38.3 57.5

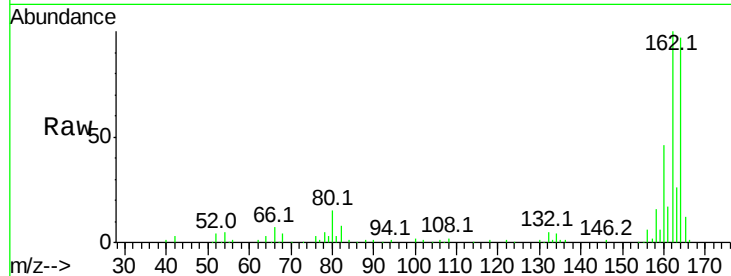


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

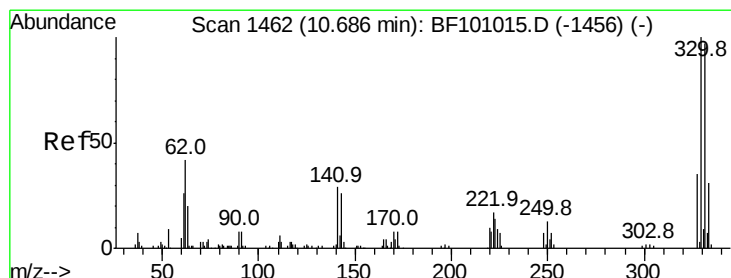
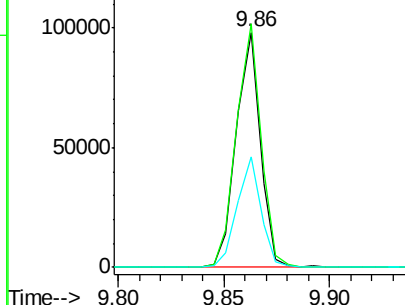



#41
 2,4,6-Tribromophenol
 Concen: 7.453 ng
 RT: 10.65 min Scan# 1456
 Delta R.T. -0.01 min
 Lab File: BF101240.D
 Acq: 8 Dec 2017 17:17

Tgt Ion:330 Resp: 6917
 Ion Ratio Lower Upper
 330 100
 332 96.2 77.0 115.6
 141 29.1 29.9 44.9#

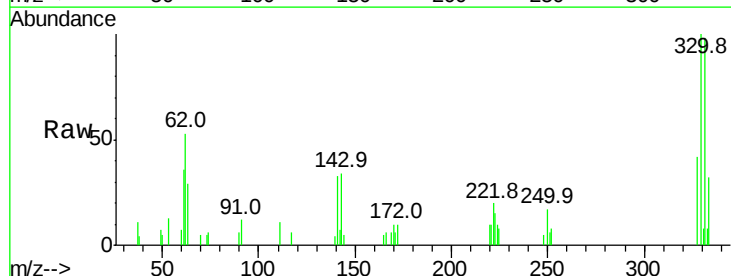

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

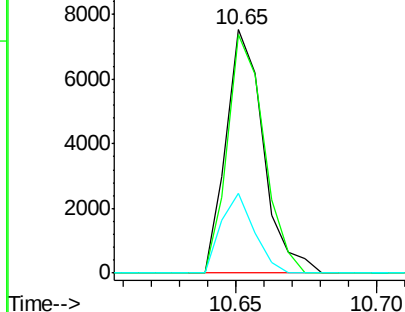


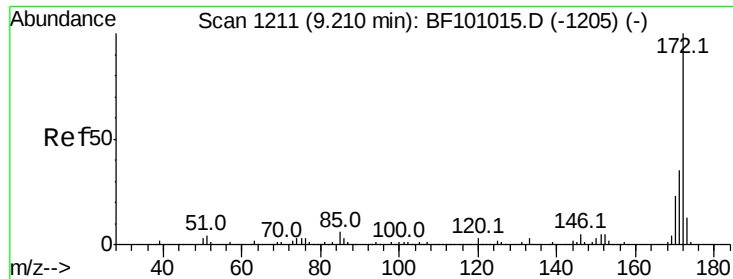




#44
 2-Fluorobiphenyl
 Concen: 7.210 ng
 RT: 9.18 min Scan# 1206
 Delta R.T. -0.01 min
 Lab File: BF101240.D
 Acq: 8 Dec 2017 17:17

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:172 Resp: 40715
 Ion Ratio Lower Upper
 172 100
 171 34.4 29.7 44.5
 170 22.1 19.6 29.4

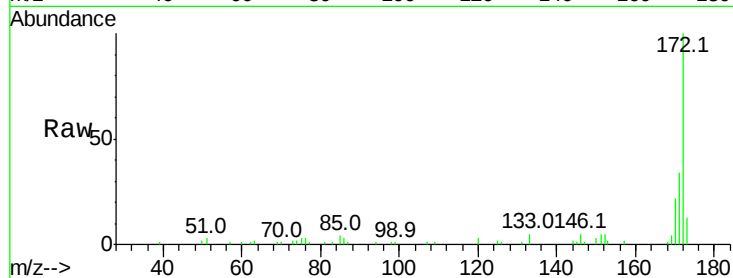


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

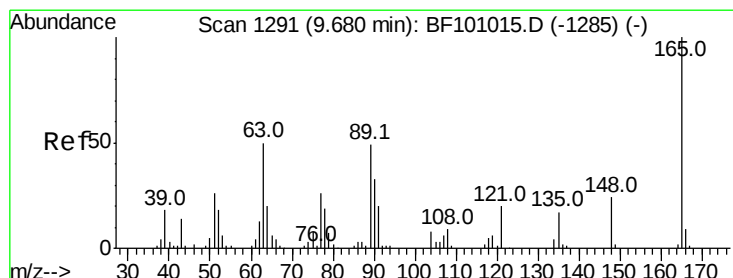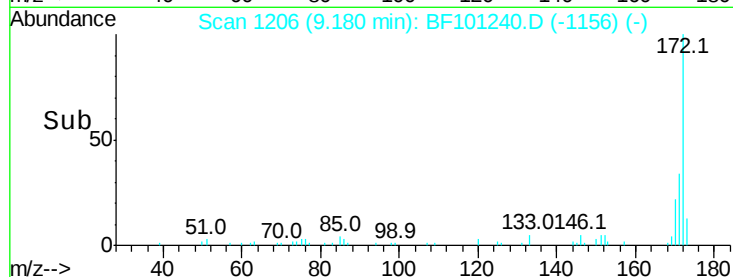
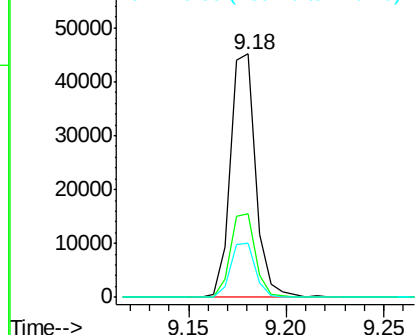



#50
 2,6-Dinitrotoluene
 Concen: 7.604 ng
 RT: 9.86 min Scan# 1322
 Delta R.T. 0.21 min
 Lab File: BF101240.D
 Acq: 8 Dec 2017 17:17

Tgt Ion:165 Resp: 9979
 Ion Ratio Lower Upper
 165 100
 63 0.0 44.7 67.1#
 89 0.0 44.0 66.0#

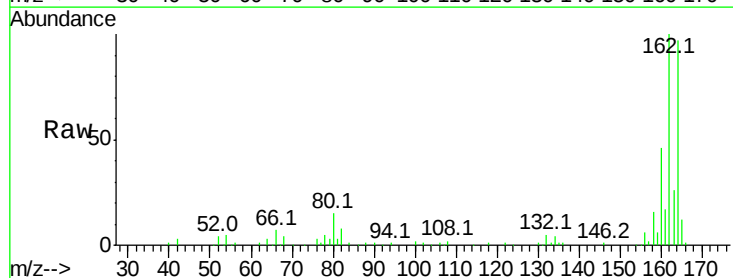

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1

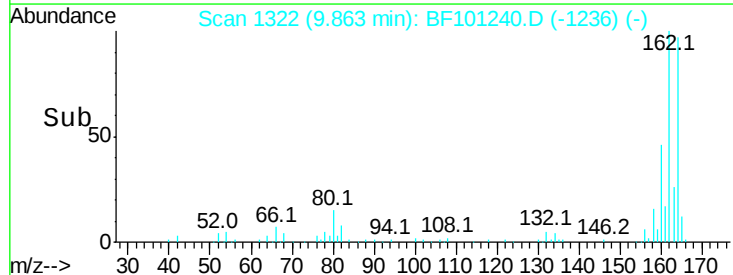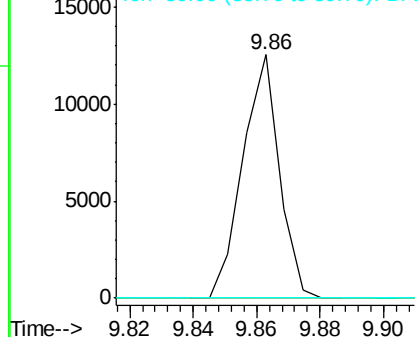







#56
 2,4-Dinitrotoluene
 Concen: 5.674 ng
 RT: 9.86 min Scan# 1322
 Delta R.T. -0.20 min
 Lab File: BF101240.D
 Acq: 8 Dec 2017 17:17

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:165 Resp: 9979
 Ion Ratio Lower Upper
 165 100
 63 0.0 36.4 54.6#
 89 0.0 57.8 86.6#
 182 0.0 1.6 2.4#

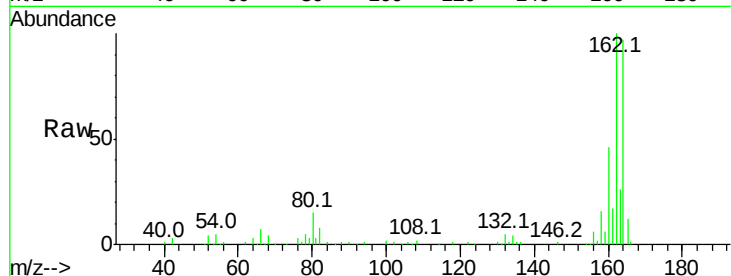


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E

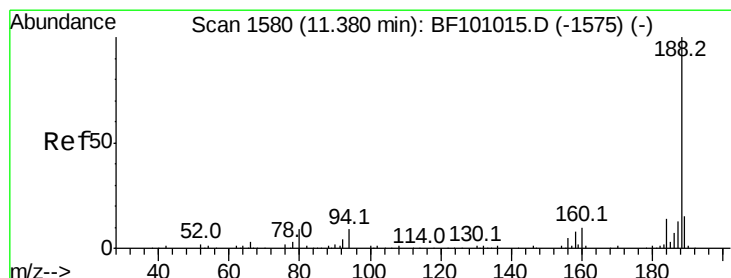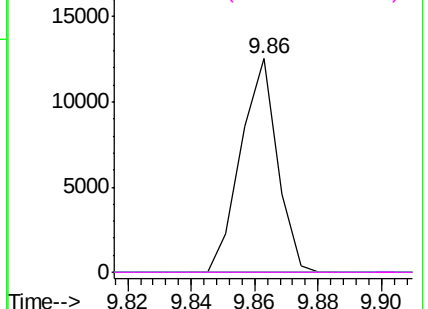




#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.35 min Scan# 1575
 Delta R.T. -0.01 min
 Lab File: BF101240.D
 Acq: 8 Dec 2017 17:17

Tgt Ion:188 Resp: 136172
 Ion Ratio Lower Upper
 188 100
 94 7.5 8.5 12.7#
 80 8.3 9.2 13.8#

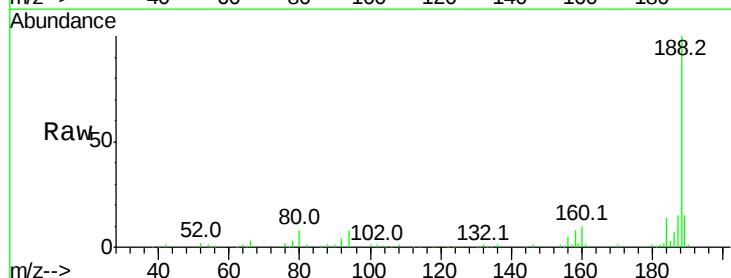

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1

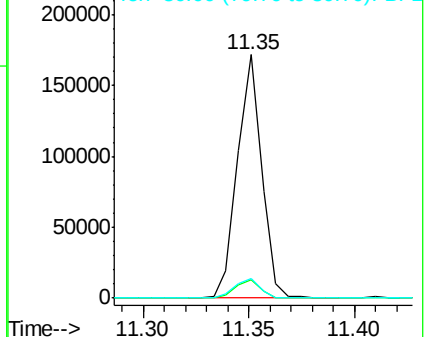

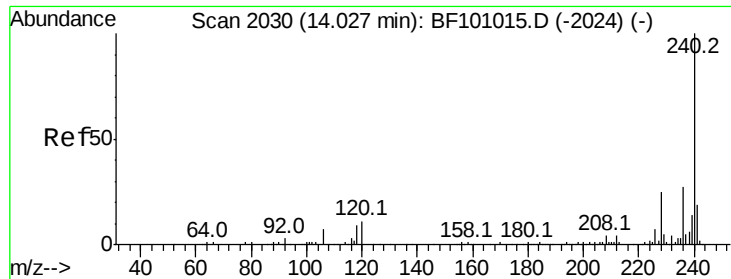

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.00 min Scan# 2025

Delta R.T. -0.01 min

Lab File: BF101240.D

Acq: 8 Dec 2017 17:17

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 99460

Ion Ratio Lower Upper

240 100

120 8.2 9.5 14.3#




236 25.1 20.7 31.1

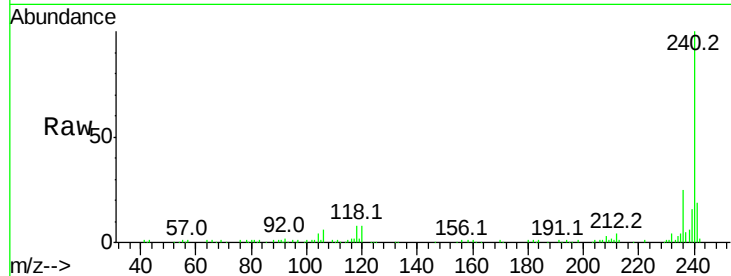

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

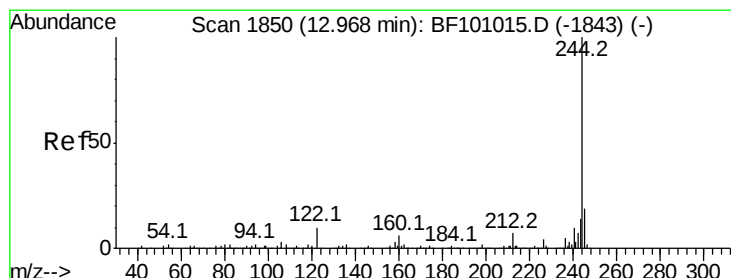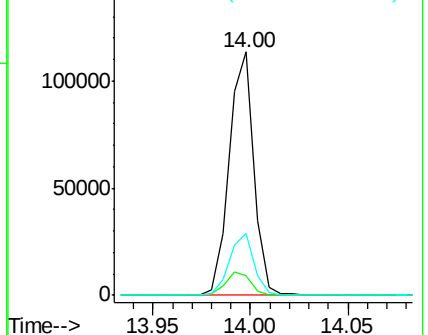

#78

Terphenyl-d14

Concen: 7.269 ng

RT: 12.93 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BF101240.D

Acq: 8 Dec 2017 17:17


Tgt Ion:244 Resp: 33055

Ion Ratio Lower Upper

244 100

212 6.0 5.4 8.0



122 7.8 11.0 16.4#

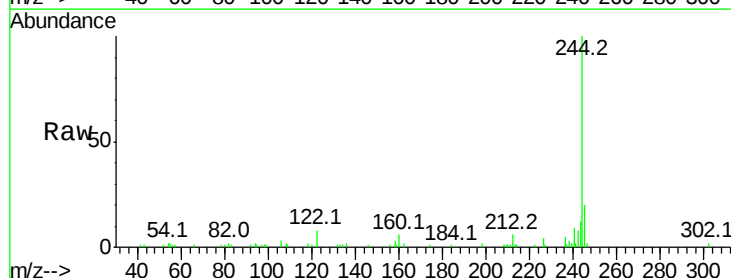


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

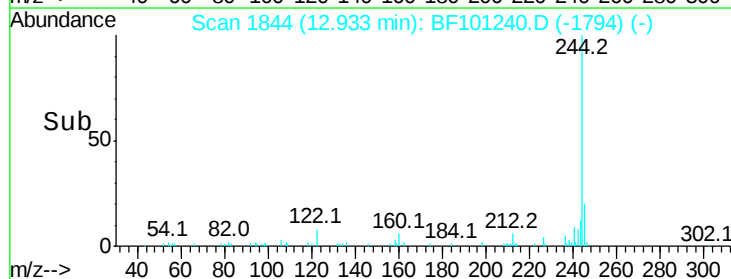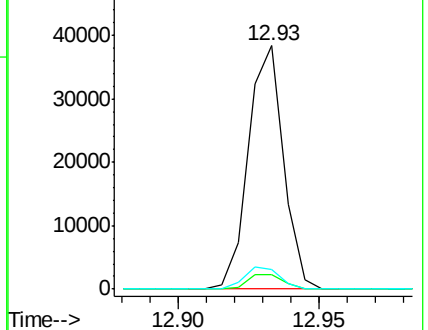

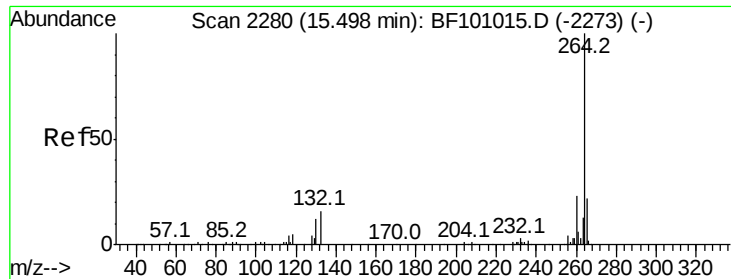

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.46 min Scan# 2274
 Delta R.T. -0.01 min
 Lab File: BF101240.D
 Acq: 8 Dec 2017 17:17

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.9	19.2	28.8
265	23.1	17.5	26.3

