

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120817\
 Data File : BF101240.D
 Acq On : 8 Dec 2017 17:17
 Operator : SJ/JU
 Sample : I6680-03 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-120617-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	566	569	582	rBV	68874	70847	20.56%	2.874%
2	6.451	739	742	753	rVB	78343	74316	21.57%	3.014%
3	6.592	763	766	772	rBB	103519	83625	24.27%	3.392%
4	6.822	802	805	810	rBV	308133	243485	70.68%	9.876%
5	6.975	828	831	837	rBB	71824	60883	17.67%	2.469%
6	7.386	898	901	909	rBB	51972	46186	13.41%	1.873%
7	8.104	1020	1023	1027	rBV	421947	324842	94.29%	13.176%
8	9.175	1202	1205	1211	rBB	116980	99907	29.00%	4.052%
9	9.863	1318	1322	1325	rBV	431980	344509	100.00%	13.973%
10	10.651	1453	1456	1461	rBB	55598	42911	12.46%	1.740%
11	11.351	1571	1575	1578	rBV	404689	322014	93.47%	13.061%
12	12.933	1840	1844	1847	rVB	91730	76951	22.34%	3.121%
13	13.780	1985	1988	1991	rBV5	4287	5753	1.67%	0.233%
14	13.821	1991	1995	1998	rBV5	5846	7553	2.19%	0.306%
15	13.998	2021	2025	2028	rBV	296319	269518	78.23%	10.932%
16	14.233	2063	2065	2070	rBV6	3718	5975	1.73%	0.242%
17	14.310	2076	2078	2079	rBV2	5330	4216	1.22%	0.171%
18	14.368	2086	2088	2092	rBV4	6048	9030	2.62%	0.366%
19	14.445	2099	2101	2103	rBV3	5453	5252	1.52%	0.213%
20	14.562	2119	2121	2123	rBV3	7069	7110	2.06%	0.288%
21	14.745	2150	2152	2155	rBV4	11392	9477	2.75%	0.384%
22	14.821	2162	2165	2169	rVB5	8707	10131	2.94%	0.411%
23	14.986	2190	2193	2194	rBV3	6063	5360	1.56%	0.217%
24	15.080	2206	2209	2215	rVB8	9812	12873	3.74%	0.522%
25	15.462	2269	2274	2280	rBV	207726	260875	75.72%	10.581%
26	15.886	2343	2346	2350	rBV6	7488	12778	3.71%	0.518%
27	16.133	2386	2388	2393	rVB5	8641	11957	3.47%	0.485%
28	16.562	2459	2461	2467	rVB7	8272	12738	3.70%	0.517%
29	16.692	2479	2483	2487	rBV6	5287	7994	2.32%	0.324%
30	18.474	2782	2786	2789	rVB5	4888	6206	1.80%	0.252%
31	18.503	2789	2791	2797	rBV7	3728	5790	1.68%	0.235%
32	18.668	2817	2819	2823	rBV5	3544	4399	1.28%	0.178%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120817\
Data File : BF101240.D
Acq On : 8 Dec 2017 17:17
Operator : SJ/JU
Sample : I6680-03 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-120617-B

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Sum of corrected areas: 2465461

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120817\
Data File : BF101240.D
Acq On : 8 Dec 2017 17:17
Operator : SJ/JU
Sample : I6680-03 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-120617-B










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.59 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.59	6.87 ng	83625	1,4-Dichlorobenzene-d4	6.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
4		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
5		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9

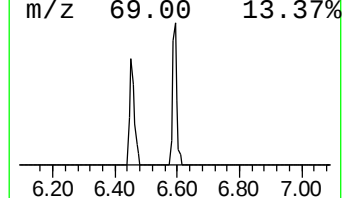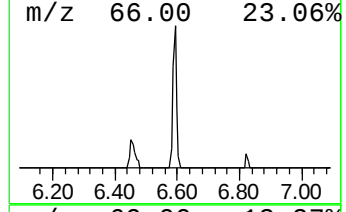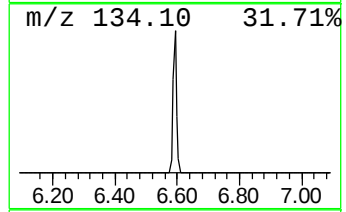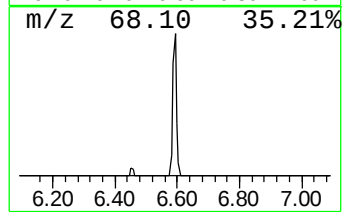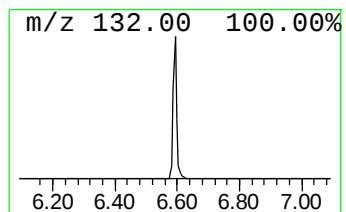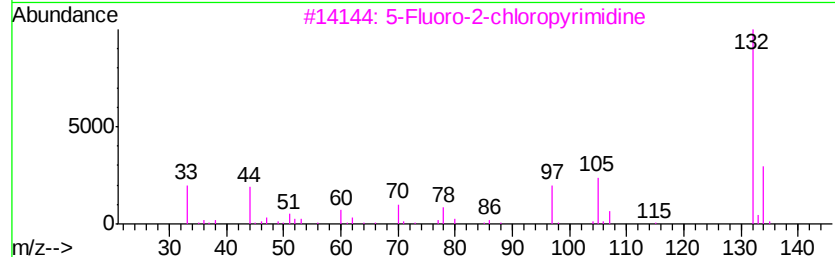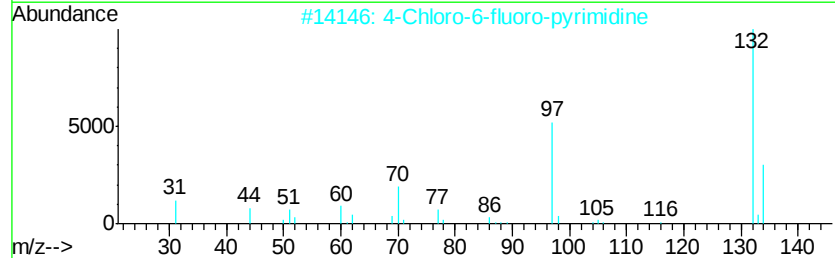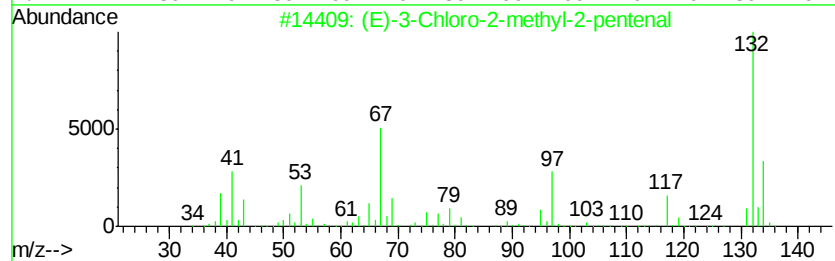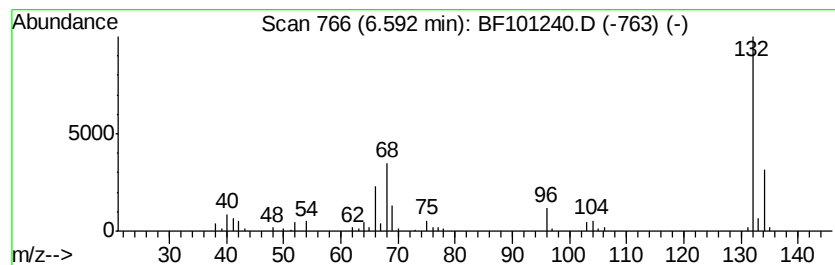

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120817\
Data File : BF101240.D
Acq On : 8 Dec 2017 17:17
Operator : SJ/JU
Sample : I6680-03 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-120617-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.59	6.59	6.9	ng	83625	1	6.82	243485	20.0