

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120817\
 Data File : BF101252.D
 Acq On : 8 Dec 2017 22:40
 Operator : SJ/JU
 Sample : I6742-01DL 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TOTES-1-4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.651	773	776	779	rBV2	184154	170057	8.12%	0.425%
2	6.827	803	806	809	rBV	336595	268366	12.81%	0.670%
3	6.880	812	815	818	rBV	166701	133192	6.36%	0.333%
4	6.980	827	832	834	rBV2	142477	169979	8.12%	0.425%
5	7.139	857	859	866	rVB2	161539	227444	10.86%	0.568%
6	7.216	866	872	875	rBV2	97826	148840	7.11%	0.372%
7	7.357	891	896	899	rBV	243274	236807	11.31%	0.592%
8	7.392	899	902	904	rVV2	195177	193263	9.23%	0.483%
9	7.433	904	909	911	rVV2	1992342	2094467	100.00%	5.232%
10	7.469	911	915	918	rVB4	104481	129810	6.20%	0.324%
11	7.510	918	922	929	rBV6	92409	188985	9.02%	0.472%
12	7.598	934	937	939	rVV2	205074	170166	8.12%	0.425%
13	7.622	939	941	945	rVB	242352	218073	10.41%	0.545%
14	7.727	957	959	961	rVV2	137478	132515	6.33%	0.331%
15	7.757	961	964	966	rVV2	147453	199096	9.51%	0.497%
16	7.780	966	968	972	rVV2	249438	265835	12.69%	0.664%
17	7.822	972	975	977	rVV2	139300	154648	7.38%	0.386%
18	7.845	977	979	982	rVV2	445070	468098	22.35%	1.169%
19	7.980	999	1002	1005	rVB2	320617	295125	14.09%	0.737%
20	8.069	1010	1017	1018	rBV3	553712	556920	26.59%	1.391%
21	8.086	1018	1020	1023	rVV2	720265	750021	35.81%	1.873%
22	8.110	1023	1024	1026	rVV	359625	334507	15.97%	0.836%
23	8.133	1026	1028	1030	rVV	522219	442934	21.15%	1.106%
24	8.163	1030	1033	1035	rVB2	384218	390658	18.65%	0.976%
25	8.192	1035	1038	1041	rBV2	154966	151207	7.22%	0.378%
26	8.398	1068	1073	1077	rVB5	290189	427983	20.43%	1.069%
27	8.451	1077	1082	1085	rBV5	108032	163826	7.82%	0.409%
28	8.492	1085	1089	1092	rBV2	257052	355700	16.98%	0.888%
29	8.527	1092	1095	1097	rBV	428408	363420	17.35%	0.908%
30	8.574	1100	1103	1107	rVB3	186790	175709	8.39%	0.439%
31	8.616	1107	1110	1112	rBV2	224873	188270	8.99%	0.470%
32	8.698	1121	1124	1128	rBV2	983880	926508	44.24%	2.314%
33	8.745	1128	1132	1133	rVV3	153516	189044	9.03%	0.472%
34	8.792	1137	1140	1143	rVV4	124576	181749	8.68%	0.454%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120817\
 Data File : BF101252.D
 Acq On : 8 Dec 2017 22:40
 Operator : SJ/JU
 Sample : I6742-01DL 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TOTES-1-4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.833	1143	1147	1149	rVB	1195157	1050171	50.14%	2.623%
36	8.927	1158	1163	1166	rBV	914166	894528	42.71%	2.234%
37	8.980	1169	1172	1173	rBV2	141869	137716	6.58%	0.344%
38	9.016	1176	1178	1182	rVB5	205926	235829	11.26%	0.589%
39	9.057	1182	1185	1189	rBV2	306242	284744	13.60%	0.711%
40	9.104	1189	1193	1194	rBV2	199771	193330	9.23%	0.483%
41	9.127	1194	1197	1200	rVB	454899	320841	15.32%	0.801%
42	9.186	1202	1207	1209	rBV2	184737	235776	11.26%	0.589%
43	9.269	1217	1221	1223	rBV	1006142	984671	47.01%	2.460%
44	9.333	1229	1232	1235	rVV2	193499	188327	8.99%	0.470%
45	9.386	1238	1241	1247	rVB	390331	437885	20.91%	1.094%
46	9.463	1249	1254	1257	rBV	769209	1077878	51.46%	2.692%
47	9.533	1262	1266	1268	rVV	1025357	1292981	61.73%	3.230%
48	9.563	1268	1271	1272	rVV	661597	698473	33.35%	1.745%
49	9.580	1272	1274	1277	rVV3	755998	850871	40.62%	2.125%
50	9.604	1277	1278	1281	rVV3	291537	225952	10.79%	0.564%
51	9.645	1281	1285	1287	rVV2	518667	514445	24.56%	1.285%
52	9.733	1297	1300	1303	rBV	372715	321751	15.36%	0.804%
53	9.798	1303	1311	1314	rBV	1290800	1287551	61.47%	3.216%
54	9.833	1314	1317	1318	rVV2	153457	143252	6.84%	0.358%
55	9.851	1318	1320	1321	rVV	221326	198081	9.46%	0.495%
56	9.868	1321	1323	1325	rVV2	301117	320983	15.33%	0.802%
57	9.904	1325	1329	1332	rVV3	210083	369013	17.62%	0.922%
58	9.933	1332	1334	1338	rVV4	192943	189401	9.04%	0.473%
59	9.974	1338	1341	1345	rVB	448328	556706	26.58%	1.391%
60	10.021	1345	1349	1352	rBV4	227736	369390	17.64%	0.923%
61	10.051	1352	1354	1355	rVV2	206720	177796	8.49%	0.444%
62	10.074	1355	1358	1361	rVV	630989	639876	30.55%	1.598%
63	10.116	1361	1365	1369	rVV2	787515	808452	38.60%	2.019%
64	10.151	1369	1371	1374	rVB	168314	127345	6.08%	0.318%
65	10.186	1374	1377	1380	rBV	367435	418646	19.99%	1.046%
66	10.216	1380	1382	1385	rVV	372978	352881	16.85%	0.881%
67	10.298	1388	1396	1398	rBV2	1366117	1580429	75.46%	3.948%
68	10.321	1398	1400	1403	rVV2	123682	136999	6.54%	0.342%
69	10.416	1410	1416	1418	rBV4	189520	310040	14.80%	0.774%
70	10.445	1418	1421	1424	rVV3	190931	286415	13.67%	0.715%
71	10.486	1426	1428	1429	rVV	222275	177574	8.48%	0.444%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120817\
Data File : BF101252.D
Acq On : 8 Dec 2017 22:40
Operator : SJ/JU
Sample : I6742-01DL 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TOTES-1-4DL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	10.510	1429	1432	1435	rVV	661992	853238	40.74%	2.131%
73	10.563	1438	1441	1443	rVV2	225421	219695	10.49%	0.549%
74	10.592	1443	1446	1450	rVV4	130464	191497	9.14%	0.478%
75	10.633	1450	1453	1456	rVV2	282507	256658	12.25%	0.641%
76	10.663	1456	1458	1461	rVV3	118064	143985	6.87%	0.360%
77	10.768	1472	1476	1485	rVB3	1257813	1999761	95.48%	4.995%
78	10.857	1489	1491	1494	rVB	142170	126917	6.06%	0.317%
79	10.957	1505	1508	1512	rBV4	207181	303072	14.47%	0.757%
80	10.998	1512	1515	1518	rVV4	295348	345844	16.51%	0.864%
81	11.051	1522	1524	1527	rVB	175489	130751	6.24%	0.327%
82	11.086	1527	1530	1532	rBV2	148270	170259	8.13%	0.425%
83	11.110	1532	1534	1540	rVB3	205679	299821	14.31%	0.749%
84	11.215	1548	1552	1554	rVV	962294	846897	40.43%	2.115%
85	11.245	1554	1557	1563	rVB2	444325	541390	25.85%	1.352%
86	11.362	1573	1577	1579	rBV	314830	308720	14.74%	0.771%
87	11.386	1579	1581	1584	rVV	241003	200195	9.56%	0.500%
88	11.480	1591	1597	1601	rBV6	172295	283161	13.52%	0.707%
89	11.521	1601	1604	1607	rVV3	124666	139757	6.67%	0.349%
90	11.592	1613	1616	1619	rVV2	159408	151932	7.25%	0.380%
91	11.639	1621	1624	1627	rVB	779493	659269	31.48%	1.647%
92	11.692	1629	1633	1639	rVB5	78248	133528	6.38%	0.334%
93	11.862	1660	1662	1665	rBV	190117	180606	8.62%	0.451%
94	11.892	1665	1667	1671	rVB2	252993	214178	10.23%	0.535%
95	12.045	1690	1693	1697	rBV	525274	429725	20.52%	1.073%
96	12.433	1757	1759	1764	rVV	329050	271903	12.98%	0.679%
97	12.804	1819	1822	1824	rVV	161059	138254	6.60%	0.345%
98	12.939	1842	1845	1848	rVB	179860	142430	6.80%	0.356%
99	14.004	2023	2026	2030	rBV	284375	263784	12.59%	0.659%
100	15.480	2273	2277	2284	rVB	164113	226694	10.82%	0.566%


Sum of corrected areas: 40034142

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120817\
Data File : BF101252.D
Acq On : 8 Dec 2017 22:40
Operator : SJ/JU
Sample : I6742-01DL 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
TOTES-1-4DL

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

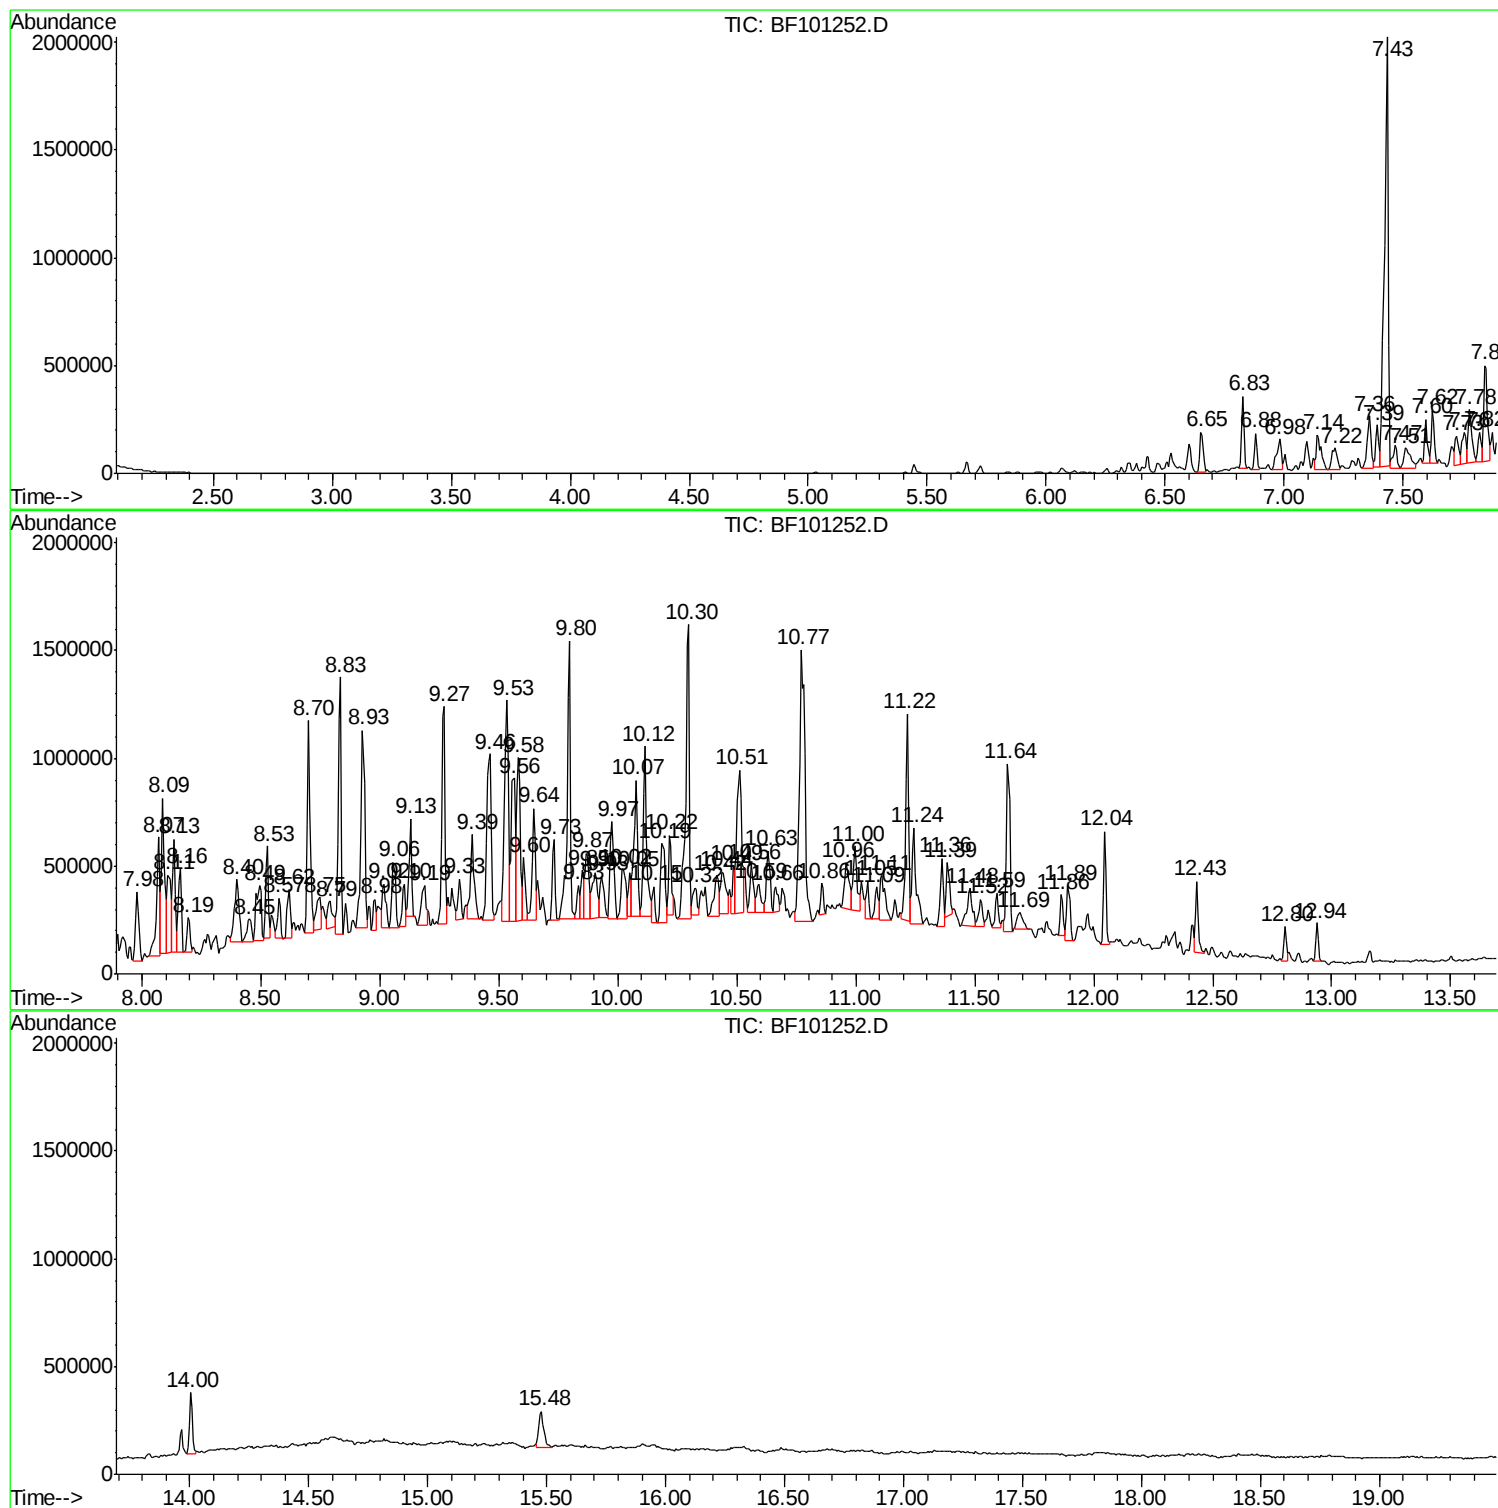

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF120817\
Data_File : BF101252.D
Acq_On : 8_Dec_2017. 22:400
Operator : SJ/JUU
Sample : I6742-01DL_10XX
Misc :
ALS_Vial : 19 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
TOTES-1-4DL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
