

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120817\
 Data File : BF101268.D
 Acq On : 9 Dec 2017 7:29
 Operator : SJ/JU
 Sample : I6744-06 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PROS-2-E(0-1)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.440	568	570	584	rBB	70739	82183	28.98%	3.958%
2	6.457	741	743	754	rBV2	75270	95538	33.68%	4.602%
3	6.598	764	767	773	rBB	105805	93460	32.95%	4.502%
4	6.828	802	806	812	rBV	273726	231647	81.67%	11.158%
5	6.981	829	832	840	rBB	87253	71613	25.25%	3.449%
6	7.386	899	901	911	rBB	41049	42008	14.81%	2.023%
7	8.110	1020	1024	1037	rBV	354267	283630	100.00%	13.661%
8	9.180	1203	1206	1211	rBV	120684	89742	31.64%	4.323%
9	9.863	1319	1322	1326	rBV	281607	255134	89.95%	12.289%
10	10.657	1454	1457	1462	rBB	35678	30852	10.88%	1.486%
11	11.357	1572	1576	1579	rBV	295832	235586	83.06%	11.347%
12	12.574	1780	1783	1786	rBV	14403	11561	4.08%	0.557%
13	12.804	1818	1822	1825	rBV	12345	10494	3.70%	0.505%
14	12.939	1841	1845	1848	rVB	85681	67173	23.68%	3.235%
15	13.751	1981	1983	1987	rBV3	2378	4011	1.41%	0.193%
16	13.827	1993	1996	1999	rBV3	4356	5076	1.79%	0.244%
17	13.921	2009	2012	2013	rBV3	4398	4466	1.57%	0.215%
18	13.968	2017	2020	2022	rVV2	10353	9778	3.45%	0.471%
19	14.004	2022	2026	2029	rVV	260536	230727	81.35%	11.113%
20	14.027	2029	2030	2035	rVB2	7035	8515	3.00%	0.410%
21	14.063	2035	2036	2039	rBV3	3047	3393	1.20%	0.163%
22	14.286	2073	2074	2076	rBV2	4644	3728	1.31%	0.180%
23	14.380	2088	2090	2092	rBV3	4181	4108	1.45%	0.198%
24	14.439	2098	2100	2102	rBV3	4457	4684	1.65%	0.226%
25	15.415	2263	2266	2271	rBV6	7152	7884	2.78%	0.380%
26	15.474	2271	2276	2281	rBV	133363	172452	60.80%	8.306%
27	15.704	2313	2315	2317	rBV2	6395	7454	2.63%	0.359%
28	17.439	2608	2610	2611	rBV2	4653	3404	1.20%	0.164%
29	17.456	2611	2613	2618	rVV6	3796	5845	2.06%	0.282%


Sum of corrected areas: 2076146

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120817\
Data File : BF101268.D
Acq On : 9 Dec 2017 7:29
Operator : SJ/JU
Sample : I6744-06 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PROS-2-E(0-1)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

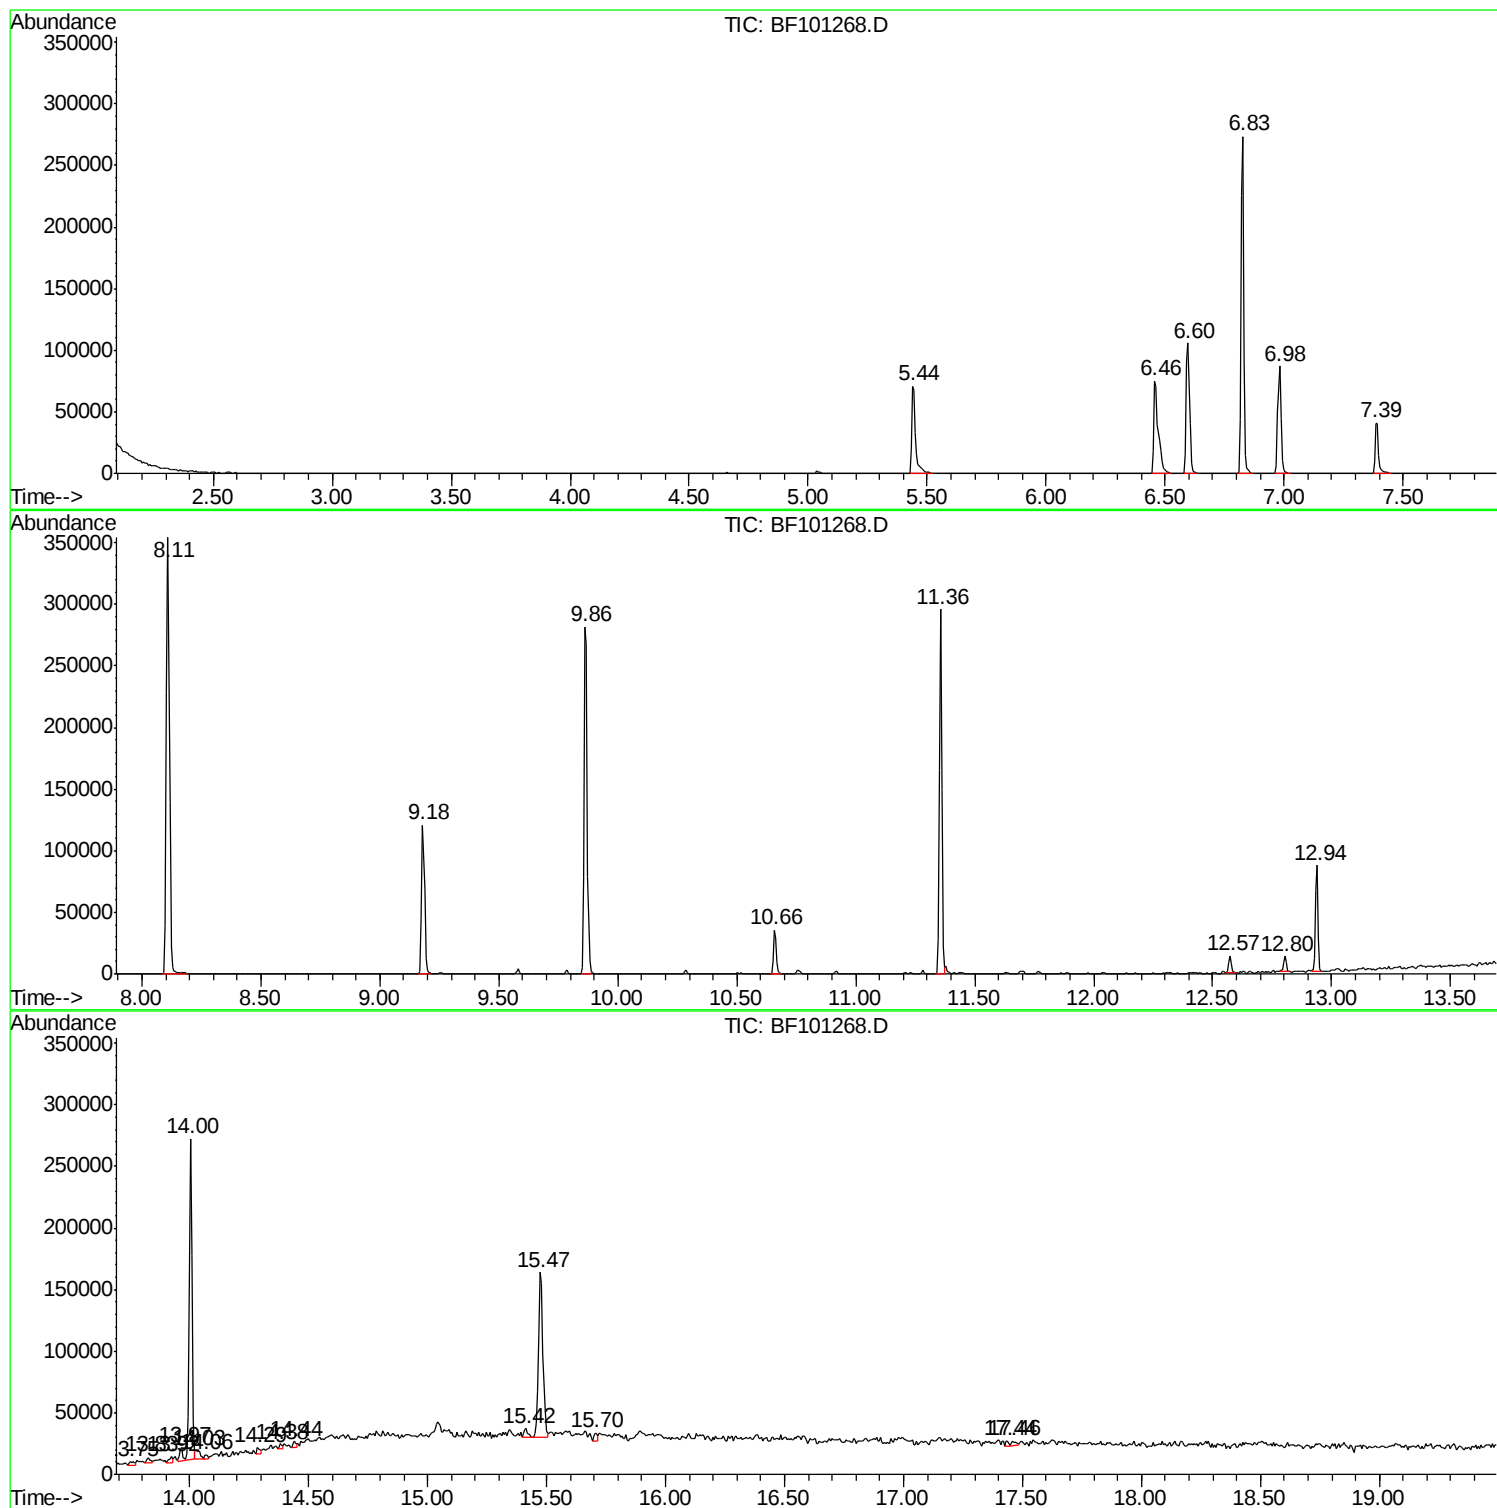

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120817\
Data File : BF101268.D
Acq On : 9 Dec 2017 7:29
Operator : SJ/JU
Sample : I6744-06 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PROS-2-E(0-1)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.60	8.07 ng	93460	1,4-Dichlorobenzene-d4	6.83

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	23
3			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
4			5-Aminoindole	132	C8H8N2	005192-03-0	10
5			Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9

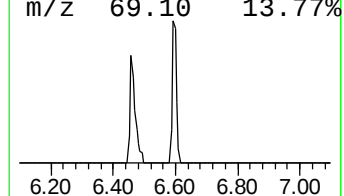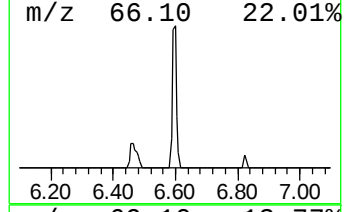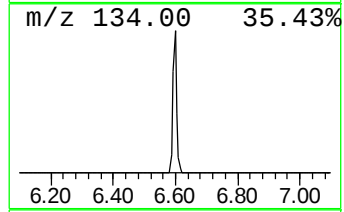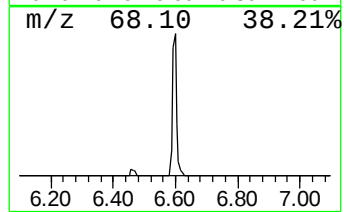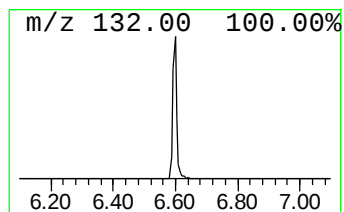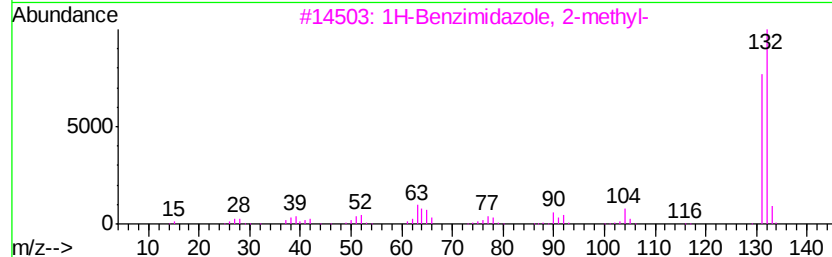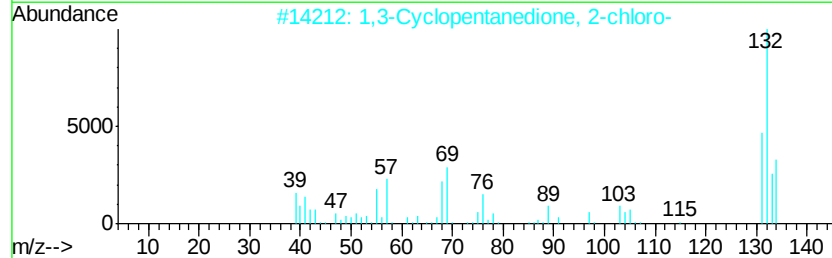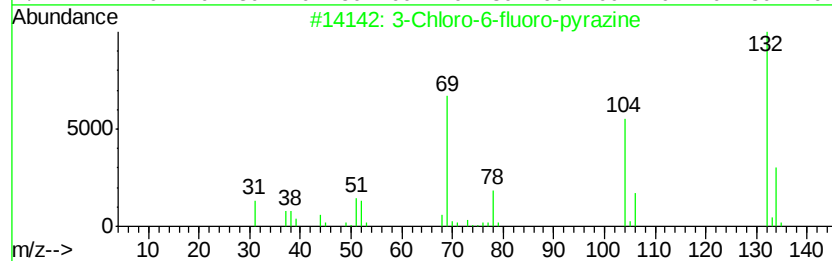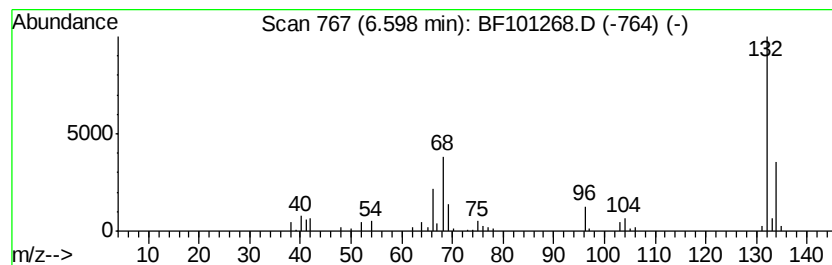

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120817\
Data File : BF101268.D
Acq On : 9 Dec 2017 7:29
Operator : SJ/JU
Sample : I6744-06 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PROS-2-E(0-1)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.60	6.60	8.1	ng	93460	1	6.83	231647	20.0